


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021219\
 Data File : VU029411.D
 Acq On : 12 Feb 2019 09:24
 Operator : JC/SP
 Sample : BFB45
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB45

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Feb 13 03:26:10 2019

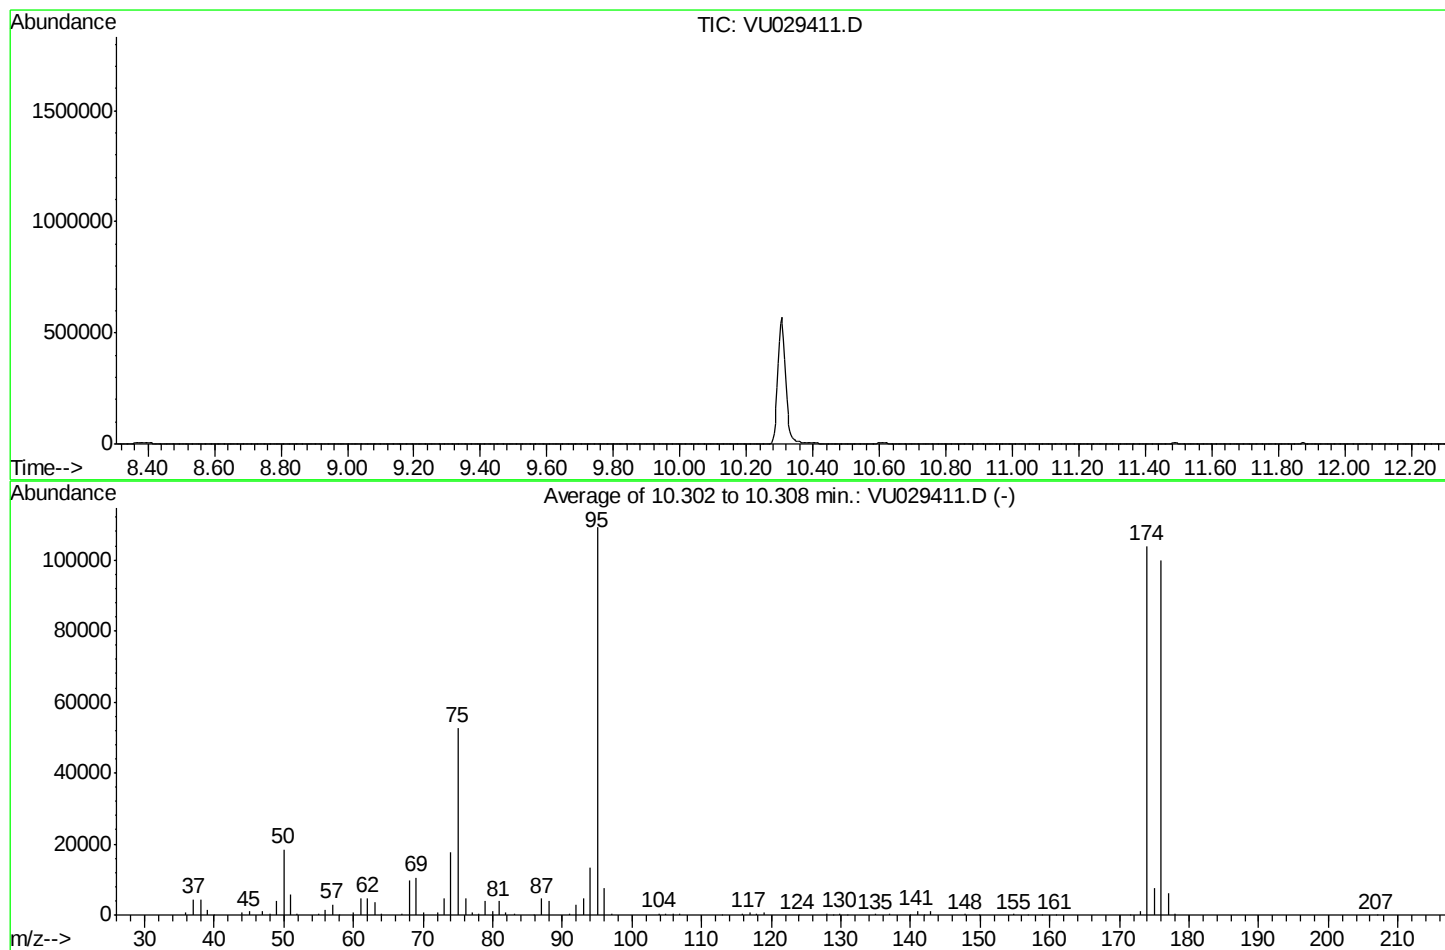

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	18576	PASS
75	95	30	80	48.3	52781	PASS
95	95	100	100	100.0	109181	PASS
96	95	5	9	7.0	7674	PASS
173	174	0.00	2	1.0	1038	PASS
174	95	50	120	95.1	103840	PASS
175	174	5	9	7.2	7437	PASS
176	174	95	101	96.1	99765	PASS
177	176	5	9	6.3	6268	PASS

Scan 2852 (10.260 min): VU029411.D
BFB45

m/z	Abundance
41.00	173.0
43.10	185.0
43.90	504.0
206.90	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.90	893.0
37.00	4615.0
38.00	4210.0
39.00	1693.0
39.90	155.0
43.00	176.0
44.00	1091.0
45.00	903.0
46.90	1072.0
48.00	525.0
49.00	4207.0
50.00	18752.0
51.00	6000.0
51.90	296.0
55.00	362.0
56.00	1621.0
57.00	3062.0
57.90	119.0
60.00	904.0
61.00	4682.0
62.00	4992.0
63.00	3517.0
64.10	349.0
67.00	345.0
68.00	9706.0
69.00	10185.0
70.00	855.0
72.00	757.0
73.00	4794.0
74.00	17376.0
75.00	52168.0
76.10	4660.0
77.00	535.0
78.00	292.0
78.90	3807.0
79.90	951.0
80.90	3790.0
81.90	808.0
83.10	218.0
85.80	125.0
87.00	4658.0
88.00	4047.0
91.00	573.0
92.00	3200.0
93.00	4497.0
94.00	13063.0
95.00	107488.0
96.00	7688.0
97.10	230.0
103.90	499.0
104.80	204.0
105.90	503.0
106.90	191.0
112.90	120.0
115.90	426.0
116.90	618.0
117.80	369.0
118.90	651.0
123.90	112.0
128.00	447.0
128.80	221.0
129.90	390.0
130.90	191.0
135.00	182.0
136.90	217.0
139.90	124.0
140.90	1190.0
142.00	160.0
142.90	1052.0
147.90	245.0
149.80	166.0
154.90	372.0
156.90	124.0
160.90	124.0
171.60	126.0
172.90	1021.0
174.00	100904.0
175.00	7227.0
176.00	94400.0
177.00	6323.0
178.00	226.0
207.10	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.90	811.0
37.00	4591.0
38.00	4393.0
39.00	1655.0
39.90	175.0
43.10	136.0
44.00	1164.0
45.00	978.0
46.90	1128.0
47.90	549.0
49.00	4181.0
50.00	19208.0
51.00	6131.0
51.90	323.0
55.00	332.0
56.00	1678.0
57.00	3129.0
57.90	127.0
59.90	878.0
61.00	4954.0
62.00	4945.0
63.00	3691.0
64.00	367.0
67.00	354.0
68.00	10171.0
69.00	10876.0
70.00	935.0
72.00	737.0
73.00	4913.0
74.00	18336.0
75.00	54600.0
76.00	4840.0
77.00	606.0
78.00	325.0
78.90	4158.0
79.90	1108.0
80.90	4156.0
81.90	938.0
83.10	280.0
85.90	105.0
87.00	4824.0
88.00	3960.0
91.00	562.0
92.00	3017.0
93.00	4742.0
94.00	13614.0
95.00	112848.0
96.00	8038.0
97.10	258.0
103.90	553.0
104.80	207.0
105.90	499.0
106.80	198.0
112.90	144.0
115.90	377.0
116.90	658.0
117.80	400.0
118.90	679.0
128.00	404.0
128.80	189.0
129.90	491.0
130.90	186.0
135.00	210.0
136.90	215.0
139.90	141.0
141.00	1291.0
141.90	172.0
142.90	1230.0
147.90	281.0
149.80	139.0
154.90	353.0
156.80	139.0
160.80	141.0
171.60	133.0
173.00	1077.0
174.00	107280.0
175.00	7685.0
176.00	102960.0
177.00	6437.0
178.00	220.0
207.10	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	705.0
37.00	4135.0
38.00	4159.0
39.00	1502.0
39.90	145.0
43.10	119.0
44.00	1172.0
45.10	881.0
46.90	1066.0
47.90	519.0
49.00	3780.0
50.00	17768.0
51.00	5522.0
52.00	266.0
55.00	369.0
56.00	1602.0
57.00	2856.0
57.90	129.0
59.90	877.0
61.00	4528.0
62.00	4558.0
63.00	3507.0
64.00	420.0
67.00	341.0
68.00	9681.0
69.00	10519.0
70.00	938.0
72.00	587.0
73.00	4604.0
74.00	17392.0
75.00	51576.0
76.00	4620.0
77.00	644.0
77.90	317.0
78.90	3971.0
79.90	1086.0
80.90	3873.0
81.90	930.0
83.10	211.0
87.00	4424.0
88.00	3764.0
91.00	460.0
92.00	2583.0
93.00	4506.0
94.00	12902.0
95.00	107208.0
96.00	7298.0
97.10	271.0
103.90	500.0
104.80	173.0
105.90	430.0
106.80	200.0
112.90	127.0
115.80	324.0
116.90	692.0
117.80	424.0
118.90	599.0
127.90	319.0
128.90	154.0
129.90	543.0
130.90	159.0
135.00	212.0
136.90	187.0
139.90	119.0
141.00	1167.0
141.90	158.0
142.90	1260.0
147.90	301.0
154.90	304.0
157.00	136.0
158.90	105.0
160.90	139.0
171.50	120.0
173.00	1017.0
174.00	103336.0
175.00	7399.0
176.00	101936.0
177.00	6045.0
178.00	186.0
207.00	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45