


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021220\
Data File : VU036735.D
Acq On : 11 Feb 2020 21:15
Operator : JC/MD
Sample : K1490-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B72

Manual Integrations
APPROVED

MMDadoda
2/12/2020 4:22:40 PM

Quant Time: Feb 12 08:47:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 12 08:13:11 2020
Response via : Initial Calibration

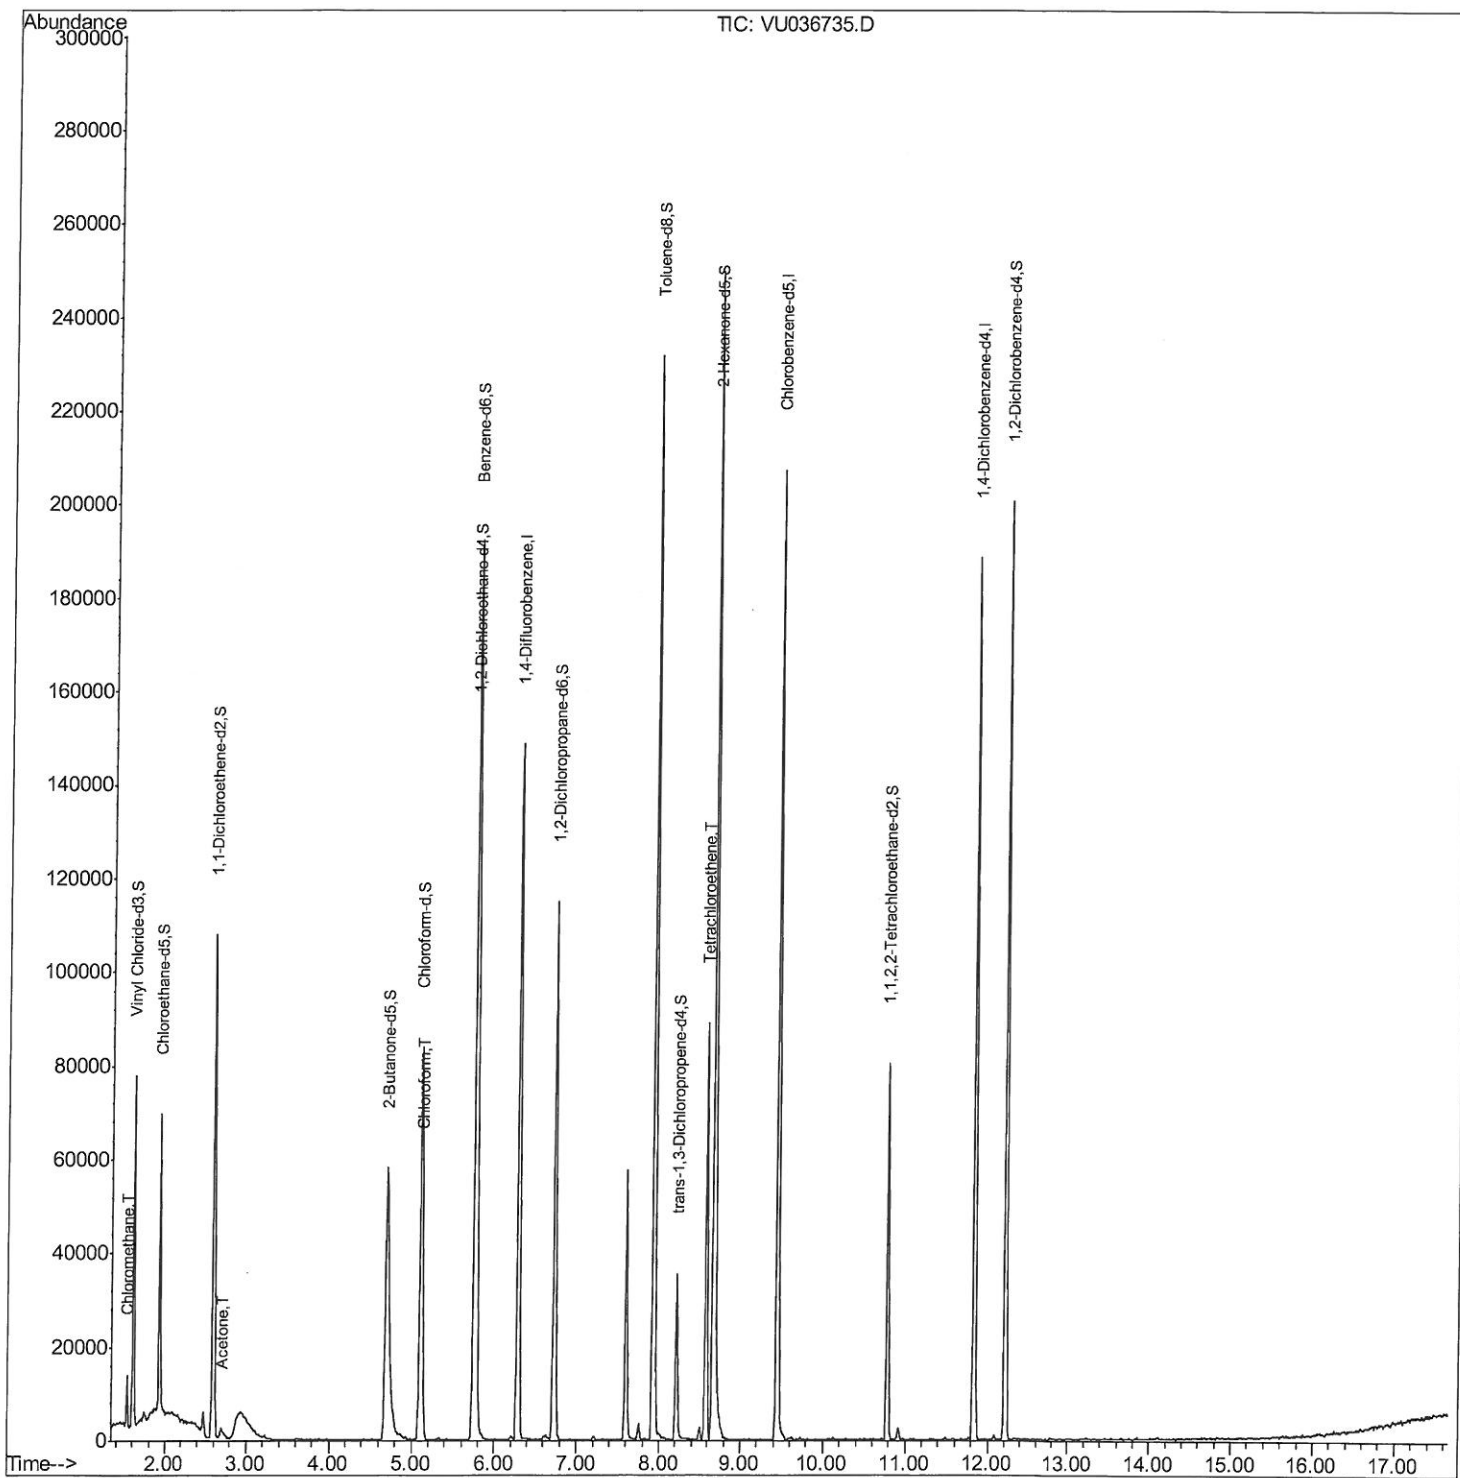

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021220\
Data File : VU036735.D
Acq On : 11 Feb 2020 21:15
Operator : JC/MD
Sample : K1490-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B72

Manual Integrations
APPROVED

MMDadoda
2/12/2020 4:22:40 PM

Quant Time: Feb 12 08:17:20 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Feb 12 08:13:11 2020
Response via : Initial Calibration

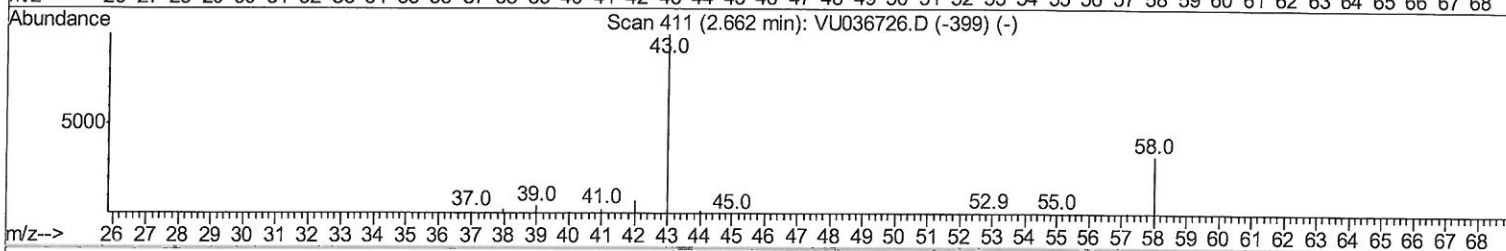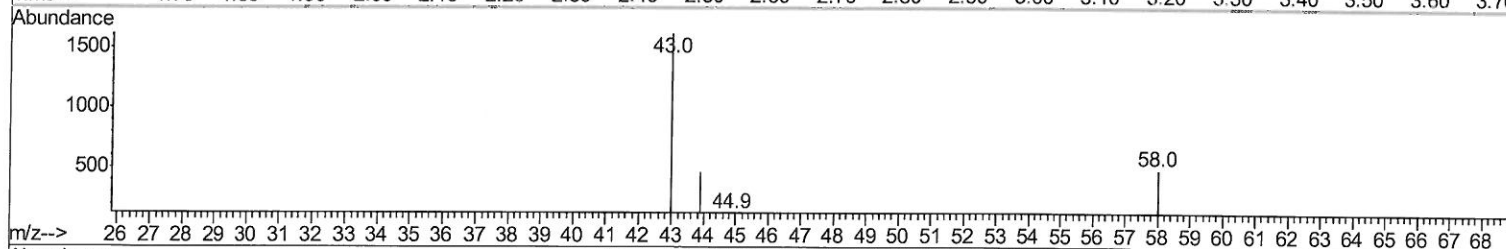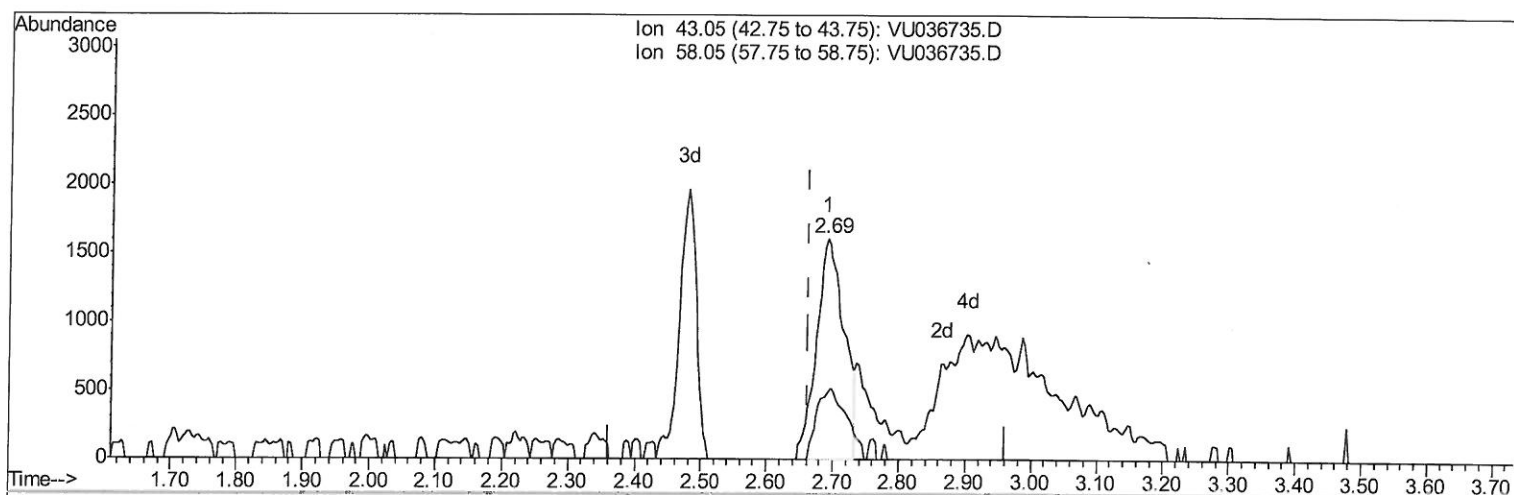

TIC: VU036735.D

(13) Acetone (T)

2.690min (+0.029) 1.74ug/L

response 4663

Ion	Exp%	Act%
43.05	100	100
58.05	32.10	34.87
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021220\
 Data File : VU036735.D
 Acq On : 11 Feb 2020 21:15
 Operator : JC/MD
 Sample : K1490-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B72

Manual Integrations
 APPROVED

MMDadoda
 2/12/2020 4:22:40 PM

Quant Time: Feb 12 08:47:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Feb 12 08:13:11 2020
 Response via : Initial Calibration

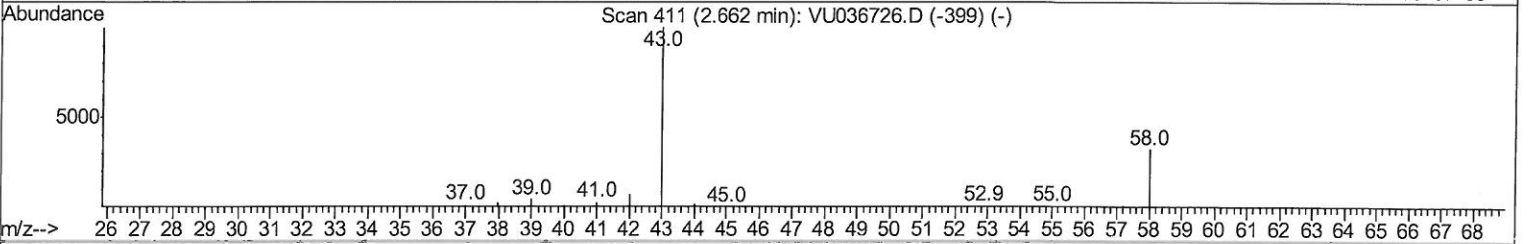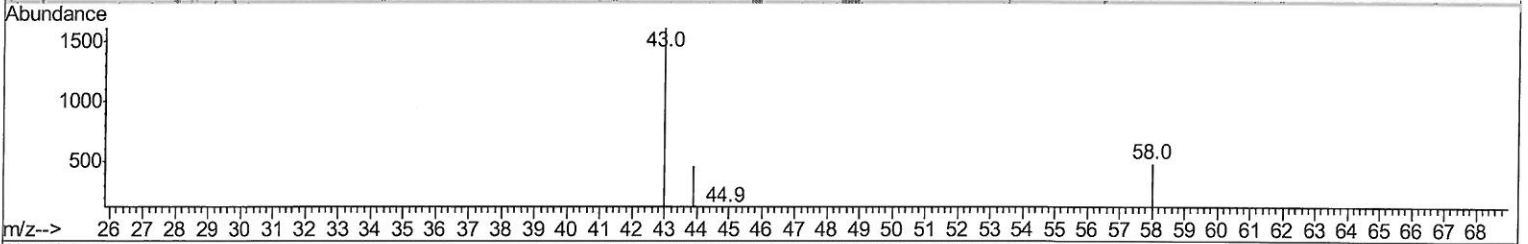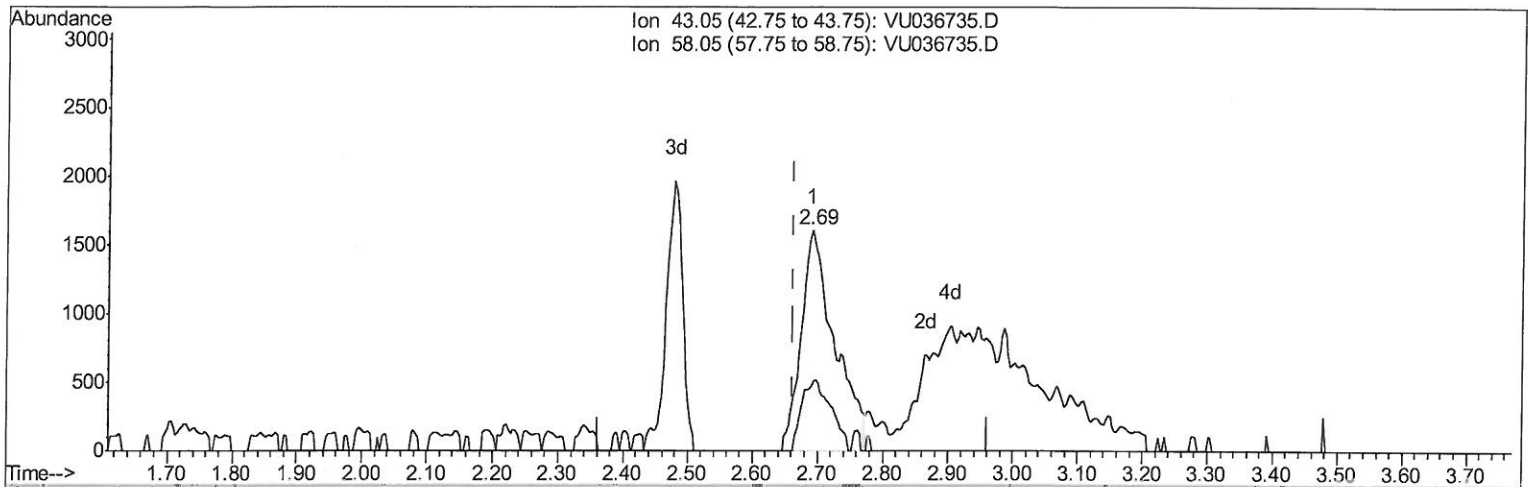

TIC: VU036735.D

(13) Acetone (T)

2.690min (+0.029) 2.14ug/L m

response 5735

Ion	Exp%	Act%
43.05	100	100
58.05	32.10	28.35
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: JMD
 2/13/20

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021220\
 Data File : VU036735.D
 Acq On : 11 Feb 2020 21:15
 Operator : JC/MD
 Sample : K1490-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B72

Manual Integrations
 APPROVED

MMDadoda
 2/12/2020 4:22:40 PM

Quant Time: Feb 12 08:47:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Feb 12 08:13:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	116182	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	109330	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	46411	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	49741	4.98	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	99.60%		
7) Chloroethane-d5	1.93	69	44809	5.17	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	103.40%		
11) 1,1-Dichloroethene-d2	2.59	63	65211	3.91	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	78.20%		
20) 2-Butanone-d5	4.70	46	115262	55.01	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	110.02%		
24) Chloroform-d	5.11	84	74891	4.86	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.20%		
26) 1,2-Dichloroethane-d4	5.74	65	44368	5.02	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	100.40%		
32) Benzene-d6	5.77	84	168728	5.07	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	101.40%		
36) 1,2-Dichloropropane-d6	6.73	67	53273	5.05	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	101.00%		
41) Toluene-d8	7.93	98	151718	4.90	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.00%		
43) trans-1,3-Dichloropropene-	8.21	79	19682	4.80	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	96.00%		
46) 2-Hexanone-d5	8.67	63	95608	51.06	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	102.12%		
57) 1,1,2,2-Tetrachloroethane-	10.78	84	39782	4.78	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	95.60%		
64) 1,2-Dichlorobenzene-d4	12.21	152	46641	5.03	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	100.60%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Chloromethane	1.53	50	7234	0.906	ug/L	95
13) Acetone	2.69	43	5735m	2.140	ug/L	
25) Chloroform	5.13	83	4524	0.277	ug/L	99
47) Tetrachloroethene	8.58	164	17654	3.022	ug/L	95

2 MD
 2/13/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed