

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021220\
 Data File : VU036757.D
 Acq On : 12 Feb 2020 18:02
 Operator : JC/MD
 Sample : L1487-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBCW2

Quant Time: Feb 13 03:25:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 13 00:59:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	123807	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	116813	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	52429	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	46246	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	1.93	69	42579	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.20%
11) 1,1-Dichloroethene-d2	2.59	63	64855	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	4.67	46	120229	53.85	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.70%
24) Chloroform-d	5.11	84	76526	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.74	65	45769	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
32) Benzene-d6	5.76	84	172879	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.73	67	56686	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.92	98	161293	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
43) trans-1,3-Dichloropropene-	8.20	79	20757	4.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.80%
46) 2-Hexanone-d5	8.66	63	104484	52.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.44%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	42457	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.60%
64) 1,2-Dichlorobenzene-d4	12.21	152	53509	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
13) Acetone	2.66	43	2611	0.914 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU021220\
Data File : VU036757.D
Acq On : 12 Feb 2020 18:02
Operator : JC/MD
Sample : L1487-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBCW2

Quant Time: Feb 13 03:25:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 13 00:59:33 2020
Response via : Initial Calibration

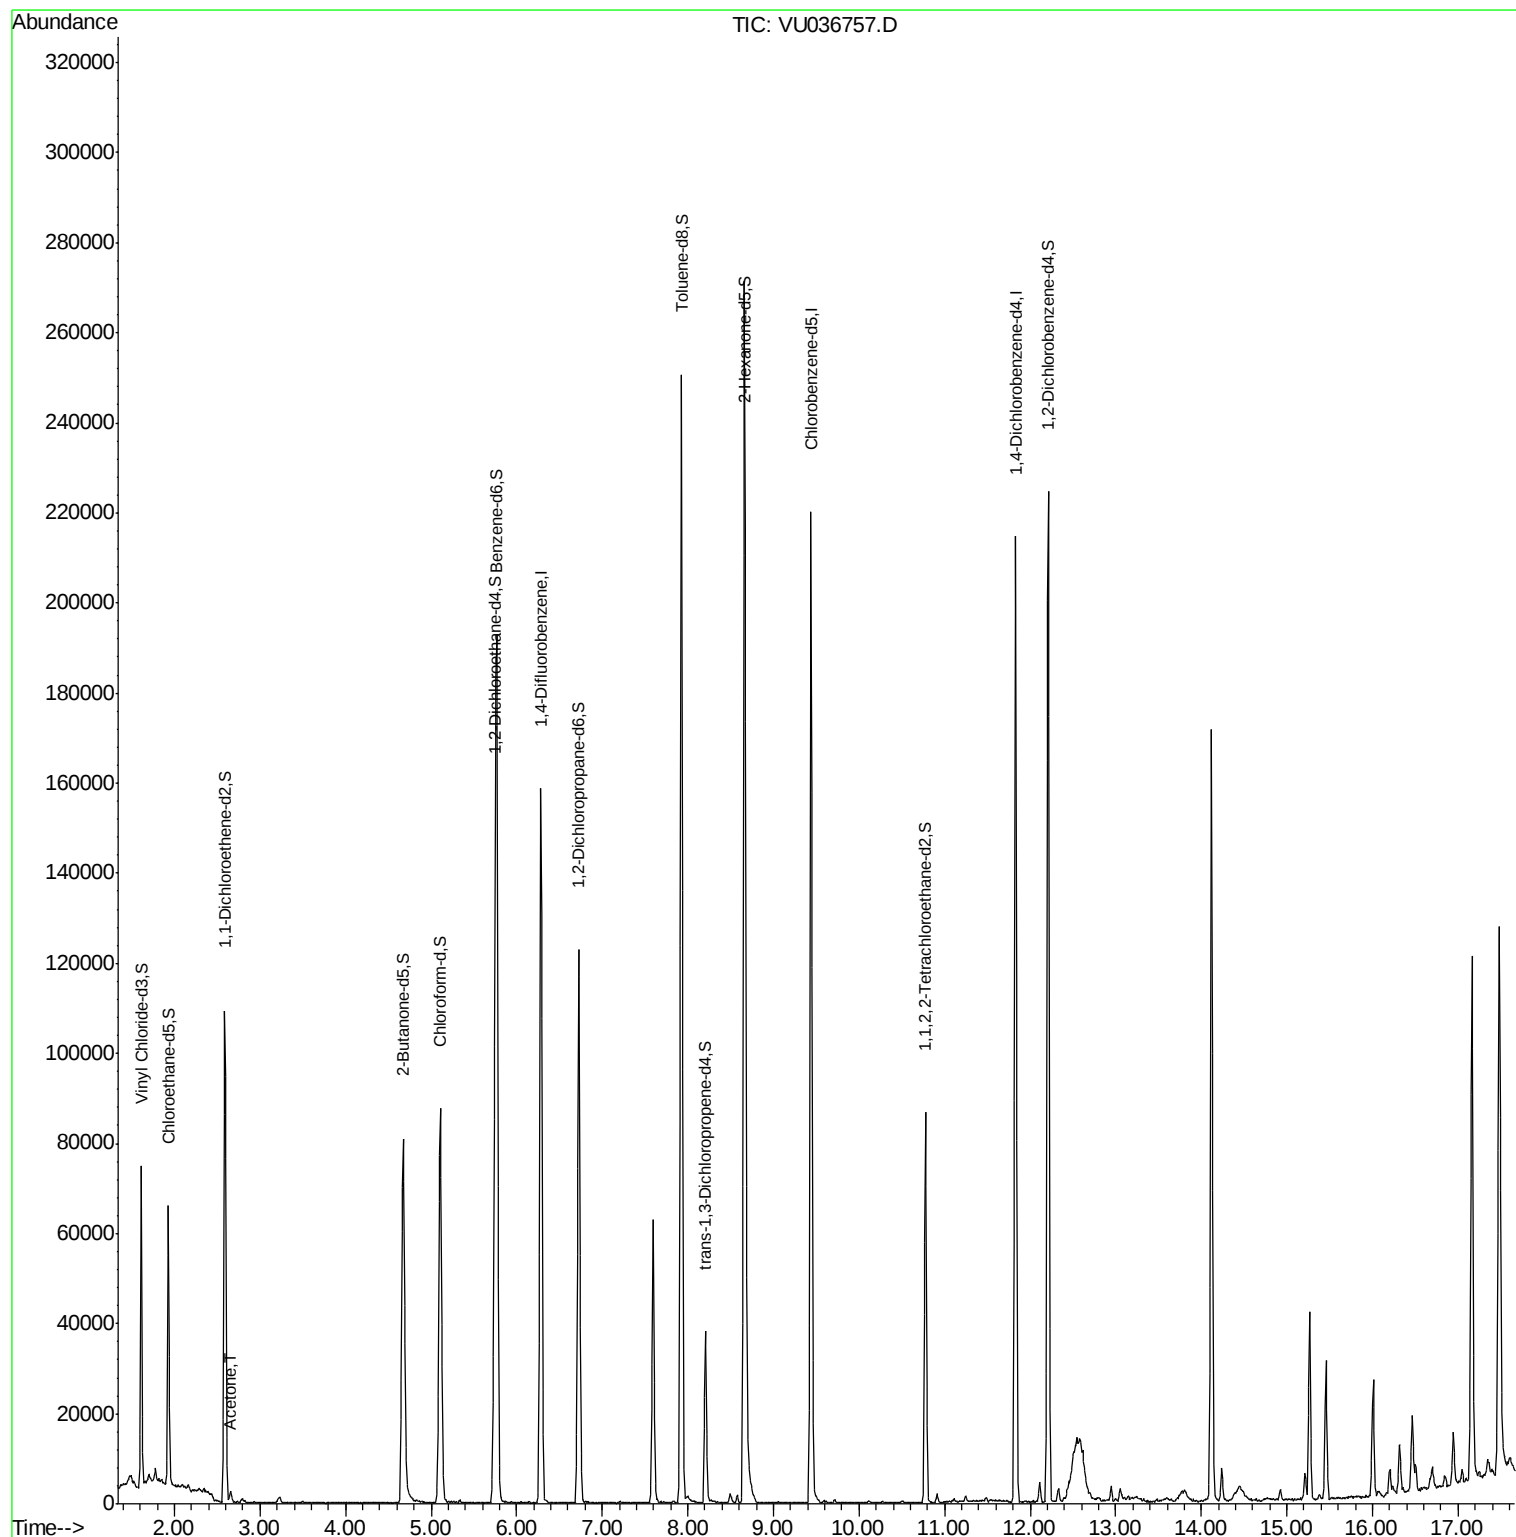

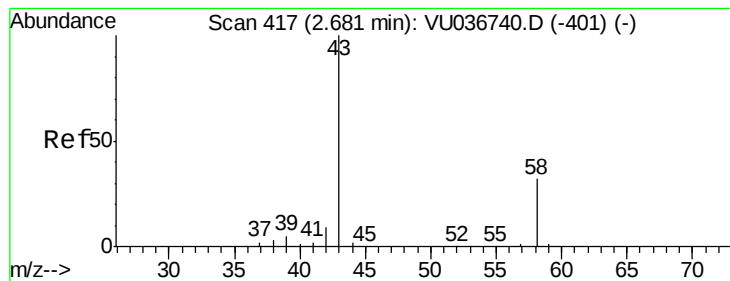

#13

Acetone

Concen: 0.914 ug/L

RT: 2.66 min Scan# 409

Delta R.T. -0.03 min

Lab File: VU036757.D

Acq: 12 Feb 2020 18:02

Instrument :

MSVOA_U

ClientSampleId :

DBCW2

Tot Ion: 43 Resp: 2611

Ion Ratio Lower Upper

43 100

58 32.9 0.0 64.2

