

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021220\
 Data File : VU036762.D
 Acq On : 12 Feb 2020 20:06
 Operator : JC/MD
 Sample : L1487-18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBCW7

Quant Time: Feb 13 03:50:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 13 00:59:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	131872	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	121479	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	56356	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	50834	4.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.60%
7) Chloroethane-d5	1.93	69	46201	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.59	63	67154	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	4.67	46	119550	50.27	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.54%
24) Chloroform-d	5.11	84	80141	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	5.74	65	46092	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
32) Benzene-d6	5.76	84	176253	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
36) 1,2-Dichloropropane-d6	6.73	67	56563	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.92	98	163431	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
43) trans-1,3-Dichloropropene-	8.20	79	21154	4.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.80%
46) 2-Hexanone-d5	8.66	63	104680	50.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.62%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	42322	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.60%
64) 1,2-Dichlorobenzene-d4	12.21	152	55708	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Ovalue
13) Acetone	2.66	43	4068	1.338 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU021220\
Data File : VU036762.D
Acq On : 12 Feb 2020 20:06
Operator : JC/MD
Sample : L1487-18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBCW7

Quant Time: Feb 13 03:50:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 13 00:59:33 2020
Response via : Initial Calibration

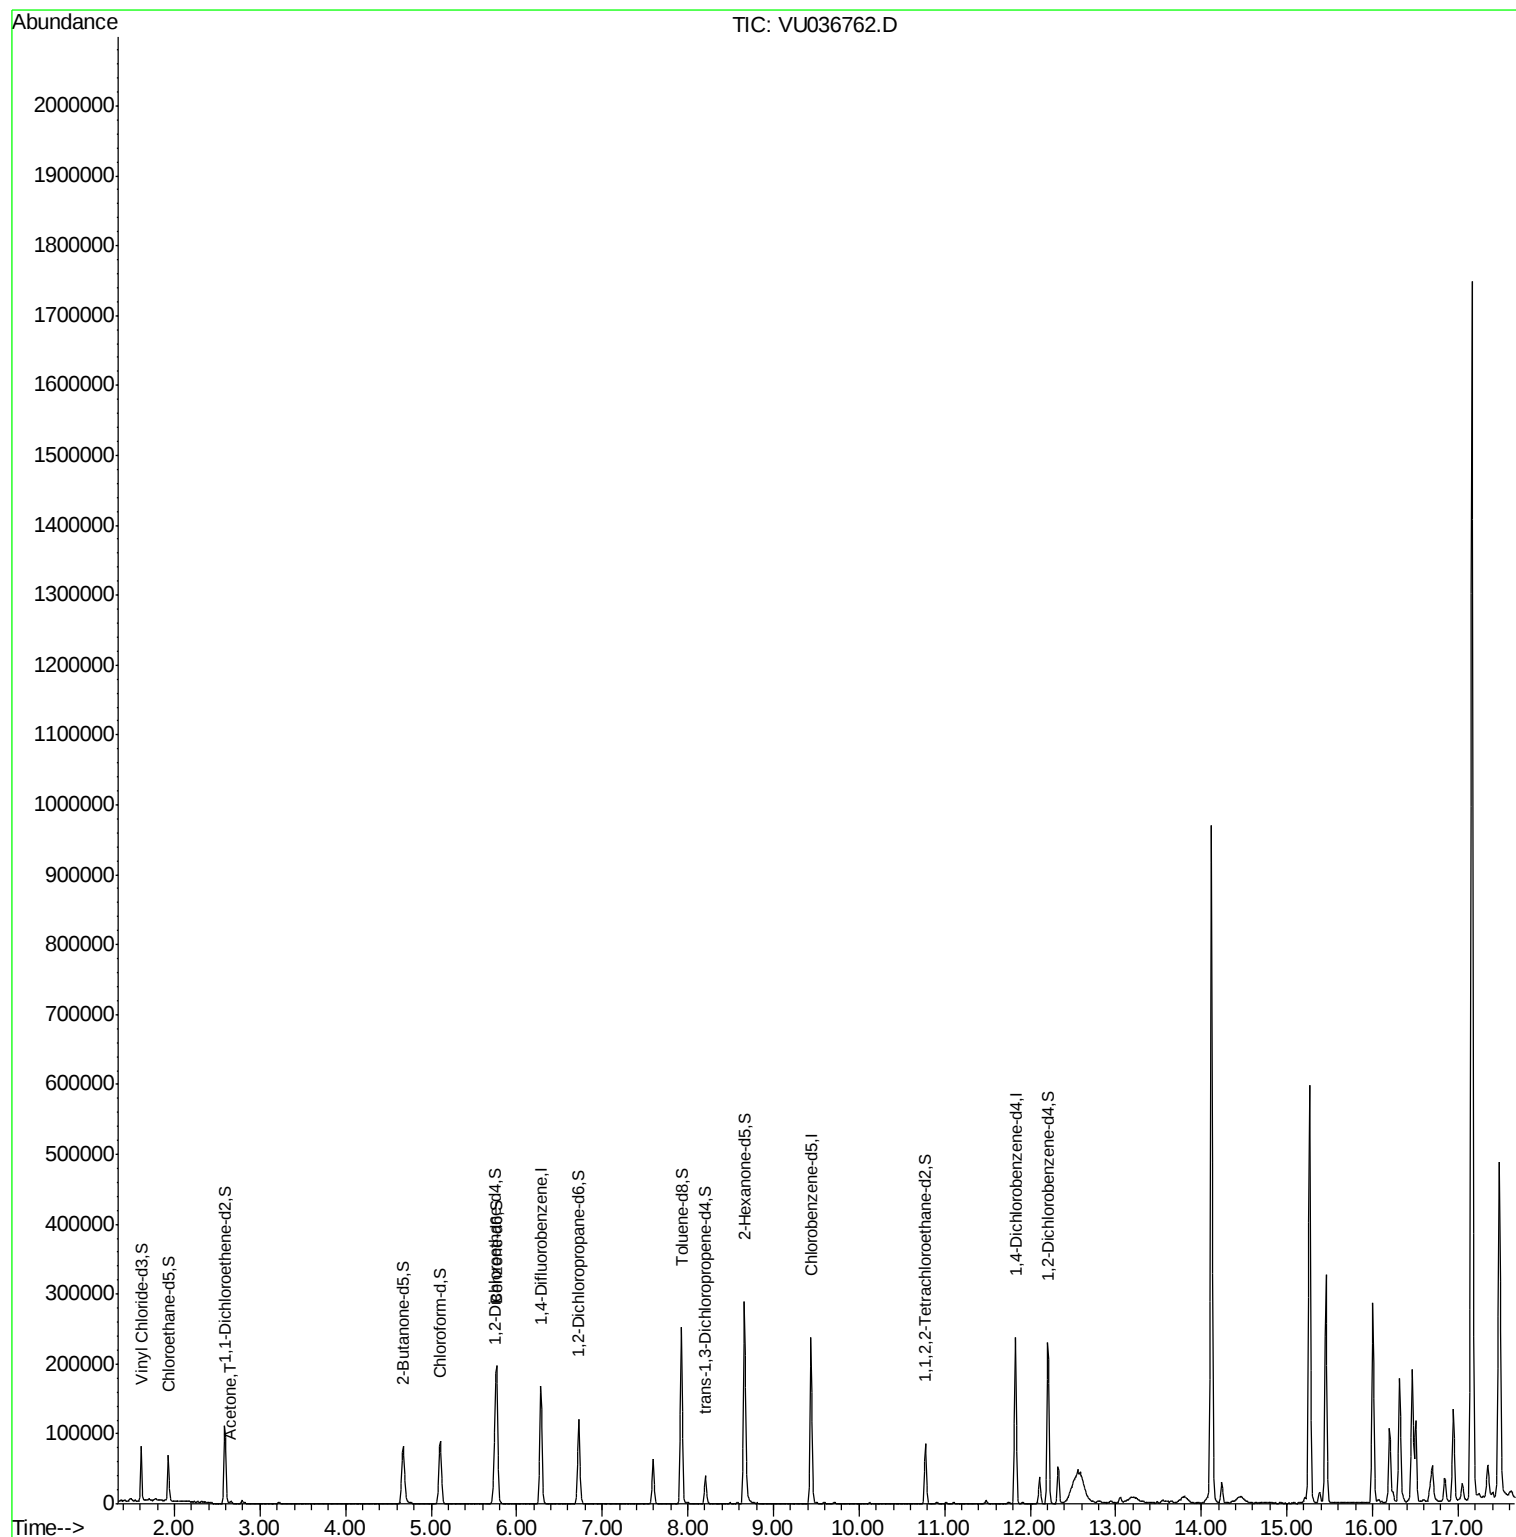

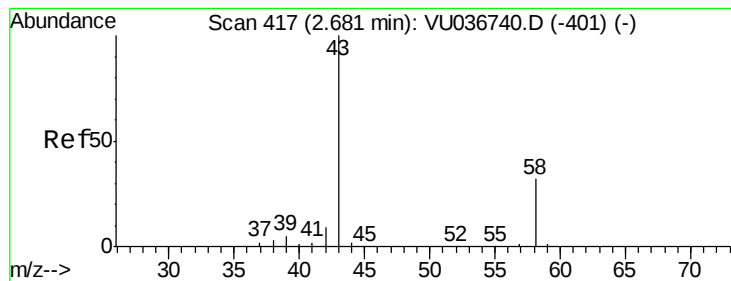

#13

Acetone

Concen: 1.338 ug/L

RT: 2.66 min Scan# 410

Delta R.T. -0.02 min

Lab File: VU036762.D

Acq: 12 Feb 2020 20:06

Instrument :
MSVOA_U
ClientSampleId :
DBCW7

Tot Ion: 43 Resp: 4068

Ion Ratio Lower Upper

43 100

58 31.4 0.0 64.2

