


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021220\
 Data File : VU036723.D
 Acq On : 11 Feb 2020 15:15
 Operator : JC/MD
 Sample : BFB04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Feb 12 08:13:11 2020

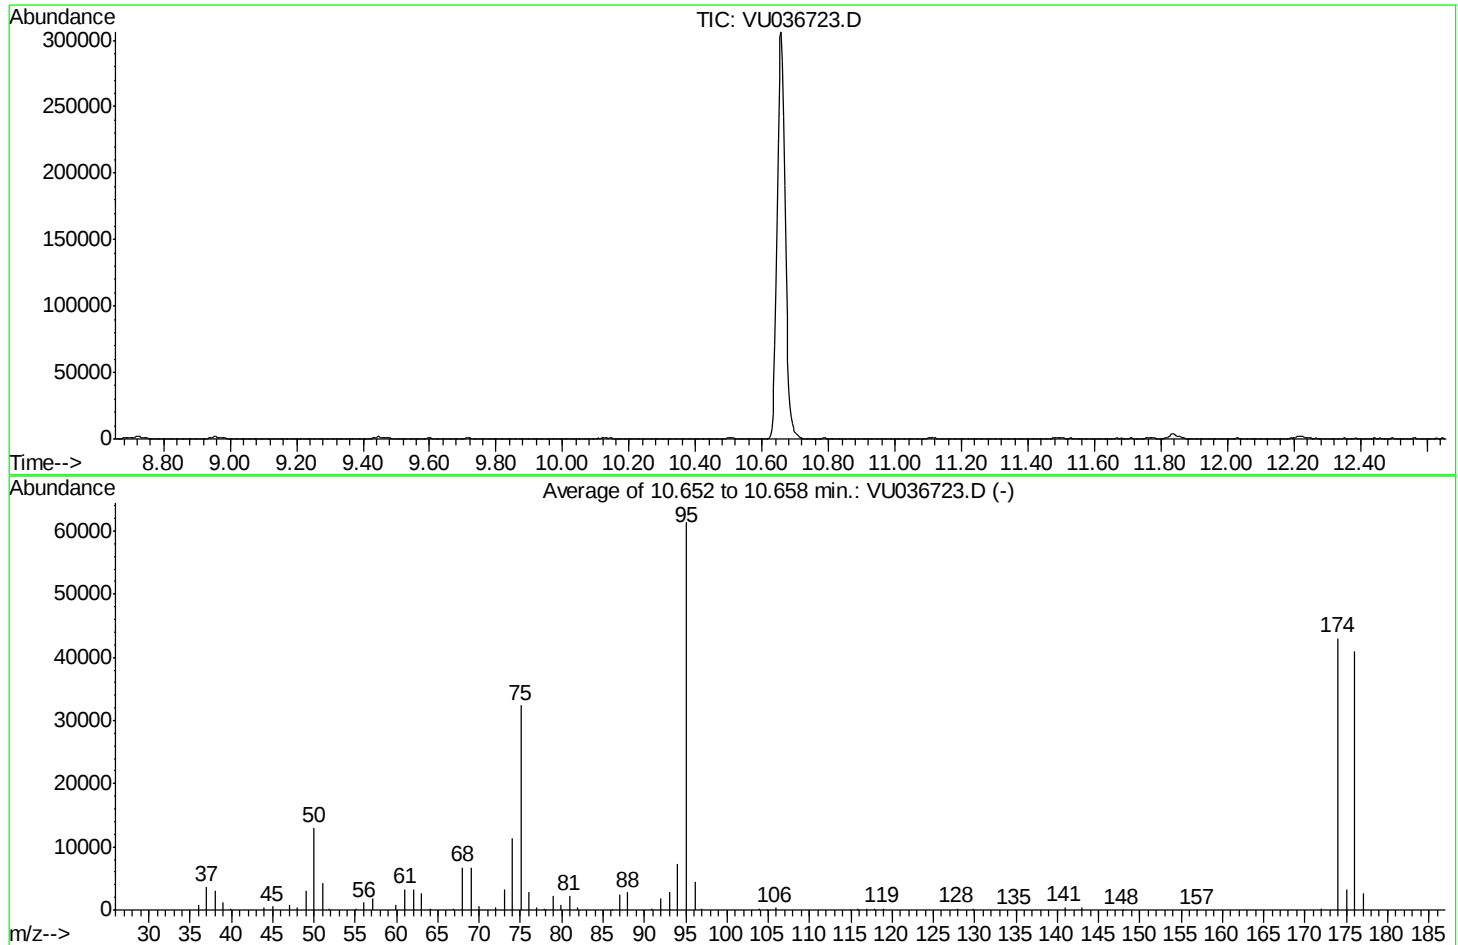

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	13044	PASS
75	95	30	80	52.8	32408	PASS
95	95	100	100	100.0	61376	PASS
96	95	5	9	7.4	4558	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.0	42970	PASS
175	174	5	9	7.5	3241	PASS
176	174	95	101	95.4	41002	PASS
177	176	5	9	6.5	2678	PASS

m/z	Abundance
44.00	412.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
35.90	738.0
37.00	3492.0
38.00	3051.0
39.00	1202.0
40.00	109.0
43.90	775.0
45.00	511.0
47.00	834.0
47.90	438.0
49.00	2929.0
50.00	12010.0
51.00	3944.0
51.90	152.0
55.00	190.0
56.10	1040.0
57.00	1835.0
59.90	803.0
61.00	3105.0
62.00	2960.0
63.00	2520.0
64.10	270.0
67.00	188.0
68.00	6119.0
69.00	6508.0
70.00	579.0
72.00	322.0
73.00	3016.0
74.00	10567.0
75.10	30304.0
76.00	2544.0
77.00	492.0
77.90	318.0
79.00	2126.0
79.90	678.0
80.90	2147.0
82.00	429.0
87.00	2367.0
88.00	2611.0
91.00	256.0
92.00	1634.0
93.00	2611.0
94.00	6726.0
95.10	57352.0
96.10	4258.0
97.00	112.0
104.00	186.0
104.90	104.0
105.90	346.0
115.90	149.0
116.90	234.0
117.90	192.0
118.90	320.0
127.90	199.0
129.80	204.0
141.00	474.0
143.00	457.0
172.00	225.0
174.00	39128.0
175.00	2888.0
176.00	37032.0
177.00	2461.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	715.0
37.00	3779.0
38.00	3147.0
39.00	1214.0
39.90	136.0
43.90	767.0
45.00	588.0
47.00	879.0
47.90	464.0
49.00	3098.0
50.00	13666.0
51.00	4354.0
51.90	185.0
55.10	192.0
56.00	1223.0
57.10	1913.0
60.00	914.0
61.00	3390.0
62.00	3487.0
63.00	2710.0
64.00	219.0
66.80	169.0
68.00	7298.0
69.00	6824.0
70.00	561.0
72.00	366.0
73.10	3364.0
74.00	11897.0
75.00	33552.0
76.00	2834.0
77.00	377.0
78.10	268.0
78.90	2421.0
80.00	849.0
80.90	2402.0
81.90	490.0
86.10	122.0
87.00	2630.0
88.00	2869.0
90.90	244.0
92.00	1844.0
93.00	2941.0
94.00	7543.0
95.10	63288.0
96.10	4673.0
97.00	152.0
103.90	237.0
105.90	356.0
114.90	106.0
115.90	225.0
117.00	271.0
117.90	245.0
118.90	276.0
127.90	238.0
129.80	199.0
134.80	124.0
140.90	485.0
143.00	467.0
147.90	118.0
157.00	103.0
172.00	197.0
174.00	45440.0
175.00	3493.0
176.00	43768.0
177.00	2841.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	766.0
37.00	3780.0
38.00	3233.0
39.00	1201.0
40.00	123.0
43.90	786.0
45.00	586.0
47.00	906.0
47.90	466.0
49.00	3173.0
50.00	13457.0
51.00	4316.0
51.90	175.0
55.00	196.0
56.10	1204.0
57.00	1971.0
59.90	884.0
61.00	3371.0
62.00	3362.0
63.00	2742.0
64.10	263.0
66.90	160.0
68.00	6903.0
69.00	6906.0
70.00	594.0
71.90	369.0
73.10	3382.0
74.00	11672.0
75.10	33368.0
76.00	2858.0
77.00	473.0
77.90	311.0
79.00	2338.0
79.90	781.0
80.90	2329.0
81.90	473.0
86.10	121.0
87.00	2596.0
88.00	2870.0
91.00	247.0
92.00	1858.0
93.00	2916.0
94.00	7543.0
95.10	63488.0
96.10	4744.0
97.00	155.0
104.00	211.0
104.90	109.0
105.90	379.0
115.90	186.0
117.00	258.0
117.90	227.0
118.90	302.0
127.90	238.0
129.80	206.0
134.90	123.0
141.00	492.0
143.00	474.0
147.90	102.0
156.90	105.0
172.00	211.0
174.00	44344.0
175.00	3344.0
176.00	42208.0
177.00	2734.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04