


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021220\
 Data File : VU036739.D
 Acq On : 12 Feb 2020 09:01
 Operator : JC/MD
 Sample : BFB05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Feb 13 00:59:33 2020

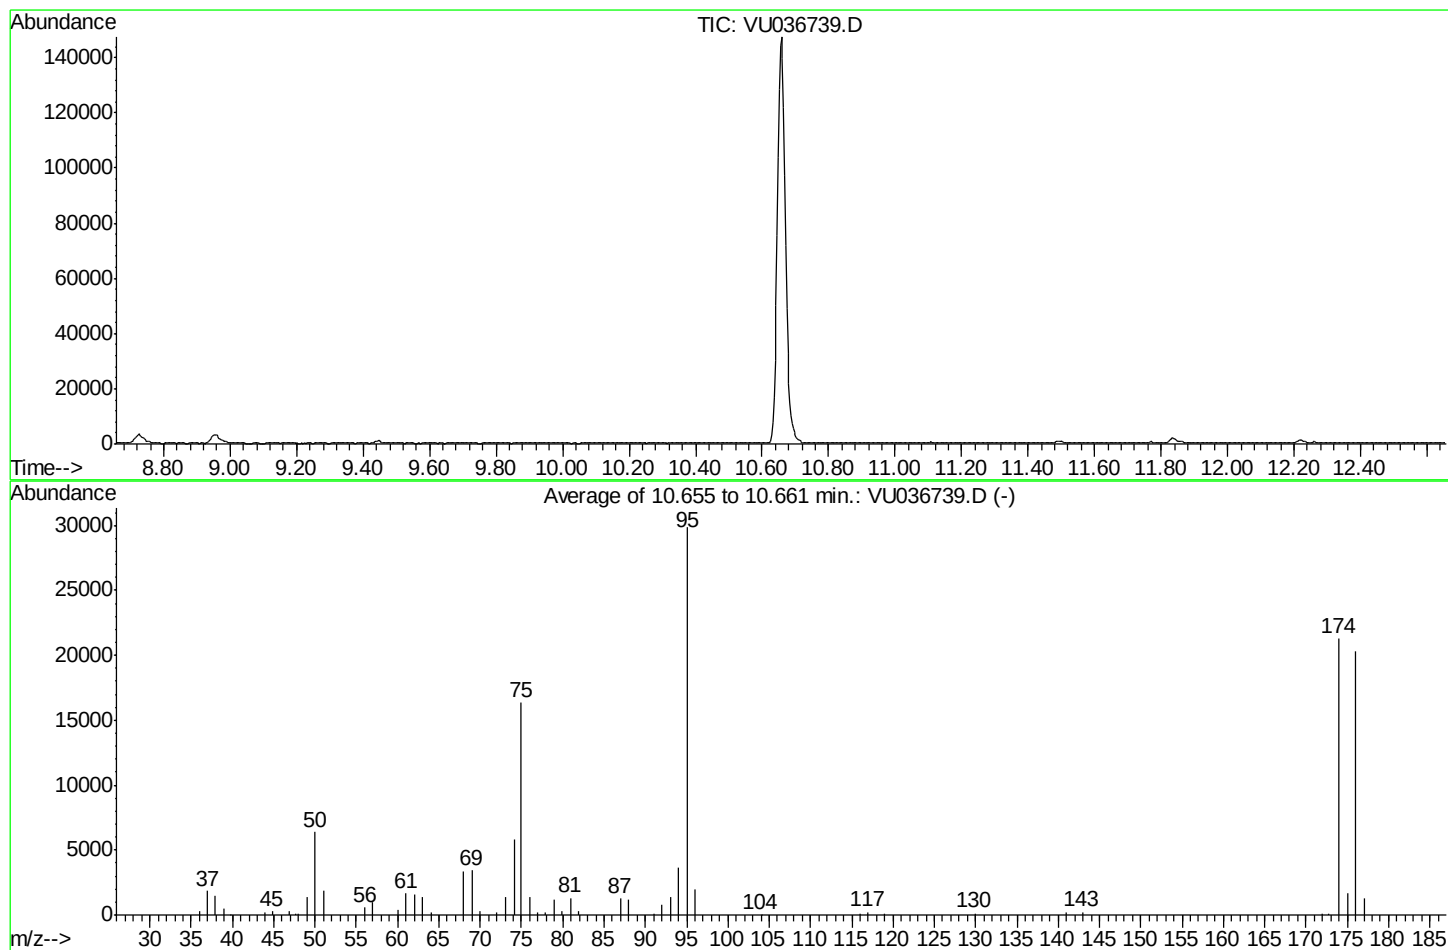

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	6404	PASS
75	95	30	80	54.8	16344	PASS
95	95	100	100	100.0	29850	PASS
96	95	5	9	6.6	1979	PASS
173	174	0.00	2	0.5	96	PASS
174	95	50	120	71.2	21248	PASS
175	174	5	9	8.0	1707	PASS
176	174	95	101	95.8	20346	PASS
177	176	5	9	6.4	1300	PASS

m/z	Abundance
35.90	333.0
37.00	1824.0
38.00	1522.0
38.90	541.0
44.10	525.0
44.80	249.0
46.90	355.0
48.00	180.0
49.00	1397.0
50.00	6550.0
51.00	1893.0
56.10	565.0
57.00	1006.0
60.00	335.0
61.00	1651.0
62.00	1631.0
63.10	1385.0
64.00	158.0
68.00	3377.0
69.00	3480.0
69.90	276.0
72.00	241.0
73.10	1474.0
74.10	6005.0
75.00	16353.0
76.00	1474.0
76.90	281.0
77.90	152.0
78.90	1183.0
79.90	314.0
80.90	1382.0
81.80	324.0
87.00	1225.0
88.00	1168.0
91.00	153.0
92.00	821.0
93.00	1325.0
94.00	3619.0
95.10	30504.0
96.00	1904.0
104.00	103.0
116.00	144.0
117.00	210.0
118.90	134.0
130.00	126.0
140.90	205.0
142.90	220.0
171.90	158.0
172.80	290.0
174.00	20552.0
175.00	1708.0
176.00	19848.0
177.00	1263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
35.90	357.0
37.00	1897.0
38.00	1522.0
39.00	512.0
44.00	536.0
44.80	273.0
46.90	340.0
47.60	181.0
49.00	1389.0
50.00	6620.0
51.00	1857.0
56.10	586.0
57.00	986.0
60.00	410.0
61.00	1734.0
62.00	1549.0
63.10	1405.0
64.00	176.0
68.00	3435.0
69.00	3554.0
69.90	265.0
72.00	209.0
73.10	1418.0
74.10	6069.0
75.00	16816.0
76.00	1454.0
77.00	260.0
77.90	187.0
78.90	1268.0
80.00	322.0
80.90	1358.0
81.80	299.0
87.00	1304.0
88.00	1219.0
91.00	155.0
92.00	807.0
93.00	1429.0
94.00	3832.0
95.10	30520.0
96.00	2035.0
115.90	138.0
117.00	214.0
118.90	144.0
130.00	126.0
140.90	165.0
142.90	232.0
171.90	118.0
174.00	21832.0
175.00	1738.0
176.00	20912.0
177.00	1329.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	331.0
37.00	1812.0
37.90	1375.0
39.00	500.0
39.80	104.0
44.00	554.0
44.90	267.0
46.90	318.0
47.80	177.0
49.00	1356.0
50.00	6042.0
51.00	1769.0
56.00	543.0
57.00	907.0
60.00	406.0
61.00	1627.0
62.00	1444.0
63.00	1295.0
64.00	161.0
68.00	3277.0
69.00	3258.0
69.90	232.0
72.00	169.0
73.10	1270.0
74.10	5485.0
75.00	15864.0
76.00	1326.0
76.90	201.0
77.90	198.0
78.90	1193.0
80.00	297.0
80.90	1145.0
81.90	226.0
87.00	1272.0
88.00	1158.0
91.00	139.0
92.00	758.0
93.00	1355.0
94.00	3639.0
95.10	28528.0
96.00	1998.0
115.90	120.0
117.00	210.0
118.90	129.0
129.90	120.0
141.00	141.0
142.90	247.0
174.00	21360.0
175.00	1675.0
176.00	20280.0
177.00	1308.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
44.00	292.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05