


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021319\
Data File : VU029437.D
Acq On : 13 Feb 2019 10:03
Operator : JC/SP
Sample : BFB46
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Feb 15 01:55:09 2019

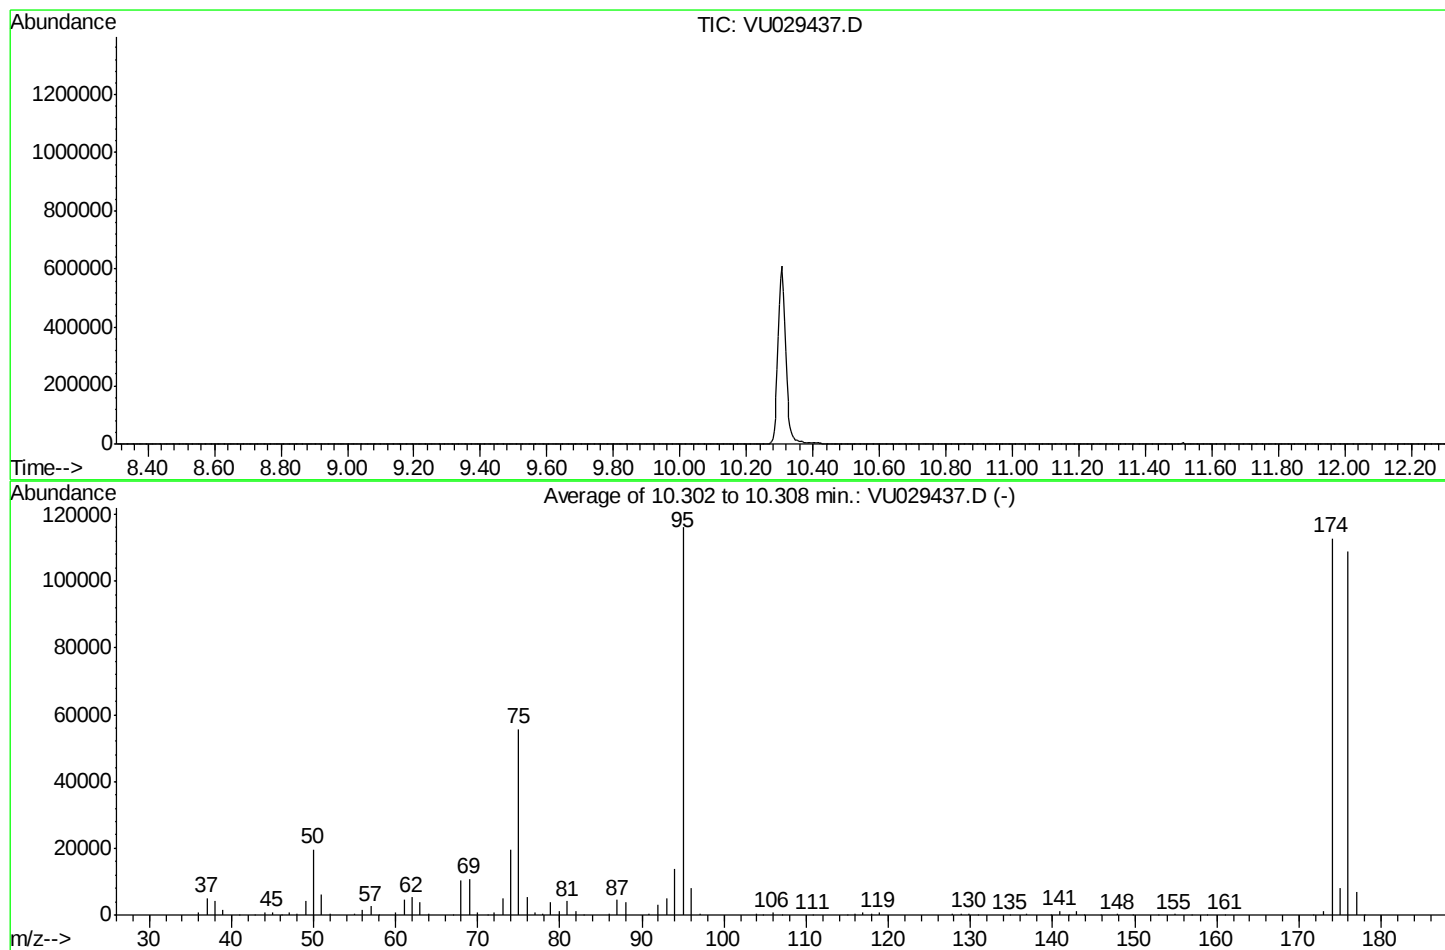

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	19600	PASS
75	95	30	80	47.9	55634	PASS
95	95	100	100	100.0	116125	PASS
96	95	5	9	6.8	7892	PASS
173	174	0.00	2	1.0	1115	PASS
174	95	50	120	97.1	112805	PASS
175	174	5	9	7.2	8169	PASS
176	174	95	101	96.5	108816	PASS
177	176	5	9	6.5	7037	PASS

m/z	Abundance
36.00	789.0
37.00	4886.0
38.00	4200.0
39.00	1679.0
39.80	151.0
40.90	158.0
42.80	111.0
44.00	1251.0
45.00	818.0
46.10	127.0
47.00	915.0
47.90	515.0
49.00	4020.0
50.00	19424.0
51.00	5803.0
52.00	257.0
55.00	391.0
56.00	1624.0
57.00	2466.0
58.00	188.0
60.00	720.0
61.00	4909.0
62.00	5219.0
63.00	3518.0
64.10	477.0
67.00	279.0
68.00	10267.0
69.00	10767.0
70.00	911.0
71.20	112.0
72.00	686.0
73.00	5176.0
74.00	19088.0
75.00	54456.0
76.00	5252.0
77.00	754.0
78.00	294.0
78.90	3901.0
79.90	1187.0
80.90	4003.0
81.90	950.0
83.00	167.0
86.00	207.0
87.00	4797.0
88.00	3914.0
90.90	493.0
92.00	3060.0
93.00	5279.0
94.00	13442.0
95.00	115688.0
96.00	7573.0
97.00	278.0
104.00	440.0
104.80	138.0
105.90	565.0
110.90	107.0
115.00	131.0
115.90	561.0
116.90	754.0
117.90	397.0
118.80	651.0
127.80	517.0
128.80	305.0
129.90	560.0
130.90	114.0
134.80	209.0
136.90	254.0
141.00	1430.0
142.00	153.0
142.90	1258.0
145.90	146.0
148.00	406.0
149.70	113.0
152.90	102.0
154.90	424.0
157.00	224.0
158.80	145.0
161.00	153.0
173.00	1174.0
174.00	115200.0
175.00	8249.0
176.00	112288.0
177.00	7014.0
178.00	186.0
207.00	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Scan 2852 (10.260 min): VU029437.D
BFB46

m/z	Abundance
40.00	142.0
44.00	501.0
67.10	128.0
207.10	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	755.0
37.00	5106.0
38.00	4183.0
39.00	1665.0
39.90	136.0
44.00	1175.0
45.00	859.0
47.10	977.0
48.00	463.0
49.00	4007.0
50.00	19200.0
51.00	5947.0
52.00	283.0
55.00	315.0
56.00	1643.0
57.00	2666.0
58.00	135.0
60.00	871.0
61.00	4603.0
62.00	5218.0
63.00	3726.0
63.90	400.0
67.00	296.0
68.00	10272.0
69.00	10831.0
70.00	989.0
72.00	604.0
73.00	4672.0
74.00	19352.0
75.00	55184.0
76.00	5153.0
77.00	726.0
77.80	447.0
78.90	3892.0
79.90	1124.0
80.90	3980.0
81.90	981.0
82.90	113.0
85.90	204.0
87.00	4327.0
88.00	3830.0
90.90	444.0
92.00	2852.0
93.00	4865.0
94.00	13361.0
95.00	112984.0
96.00	7925.0
97.00	296.0
104.00	481.0
104.80	121.0
105.90	631.0
107.00	102.0
110.80	158.0
115.00	103.0
115.90	404.0
116.90	693.0
117.90	444.0
118.90	780.0
127.90	394.0
128.90	193.0
129.80	489.0
130.80	177.0
134.80	182.0
136.80	232.0
139.80	102.0
140.90	1165.0
141.90	177.0
142.90	1220.0
143.80	106.0
145.90	220.0
147.90	333.0
152.90	116.0
154.90	331.0
156.90	185.0
158.90	128.0
171.70	258.0
173.00	1057.0
174.00	106448.0
175.00	7778.0
176.00	101568.0
177.00	6848.0
177.90	170.0
207.00	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	814.0
37.00	5329.0
38.00	4348.0
39.00	1750.0
39.80	140.0
40.90	146.0
42.80	100.0
44.00	1263.0
45.00	841.0
46.00	107.0
47.00	930.0
47.90	517.0
49.00	4271.0
50.00	20176.0
51.00	6274.0
52.00	280.0
55.00	372.0
56.00	1689.0
57.00	2658.0
57.90	200.0
60.00	799.0
61.00	4894.0
62.00	5400.0
63.00	3820.0
64.00	468.0
67.00	315.0
68.00	10664.0
69.00	11085.0
70.00	1007.0
72.00	660.0
73.00	5251.0
74.00	20200.0
75.00	57264.0
76.00	5394.0
77.00	808.0
77.90	416.0
78.90	4154.0
79.90	1235.0
80.90	4155.0
81.90	1052.0
83.00	138.0
86.00	231.0
87.00	4669.0
88.00	3981.0
90.90	485.0
92.00	3007.0
93.00	5414.0
94.00	14120.0
95.00	119704.0
96.00	8180.0
97.00	303.0
104.00	509.0
104.70	132.0
105.90	663.0
110.80	144.0
115.00	140.0
115.90	506.0
116.90	700.0
117.90	427.0
118.90	768.0
127.90	485.0
128.80	271.0
129.80	530.0
130.80	160.0
134.80	196.0
136.90	250.0
139.80	103.0
141.00	1336.0
141.90	180.0
142.90	1316.0
143.80	106.0
145.90	188.0
147.90	407.0
152.80	122.0
154.90	387.0
156.90	202.0
158.70	146.0
161.00	132.0
171.70	249.0
173.00	1115.0
174.00	116768.0
175.00	8482.0
176.00	112592.0
177.00	7251.0
178.00	165.0
207.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46