


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021320\
 Data File : VU036764.D
 Acq On : 13 Feb 2020 11:08
 Operator : JC/MD
 Sample : BFB06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Feb 14 00:15:45 2020

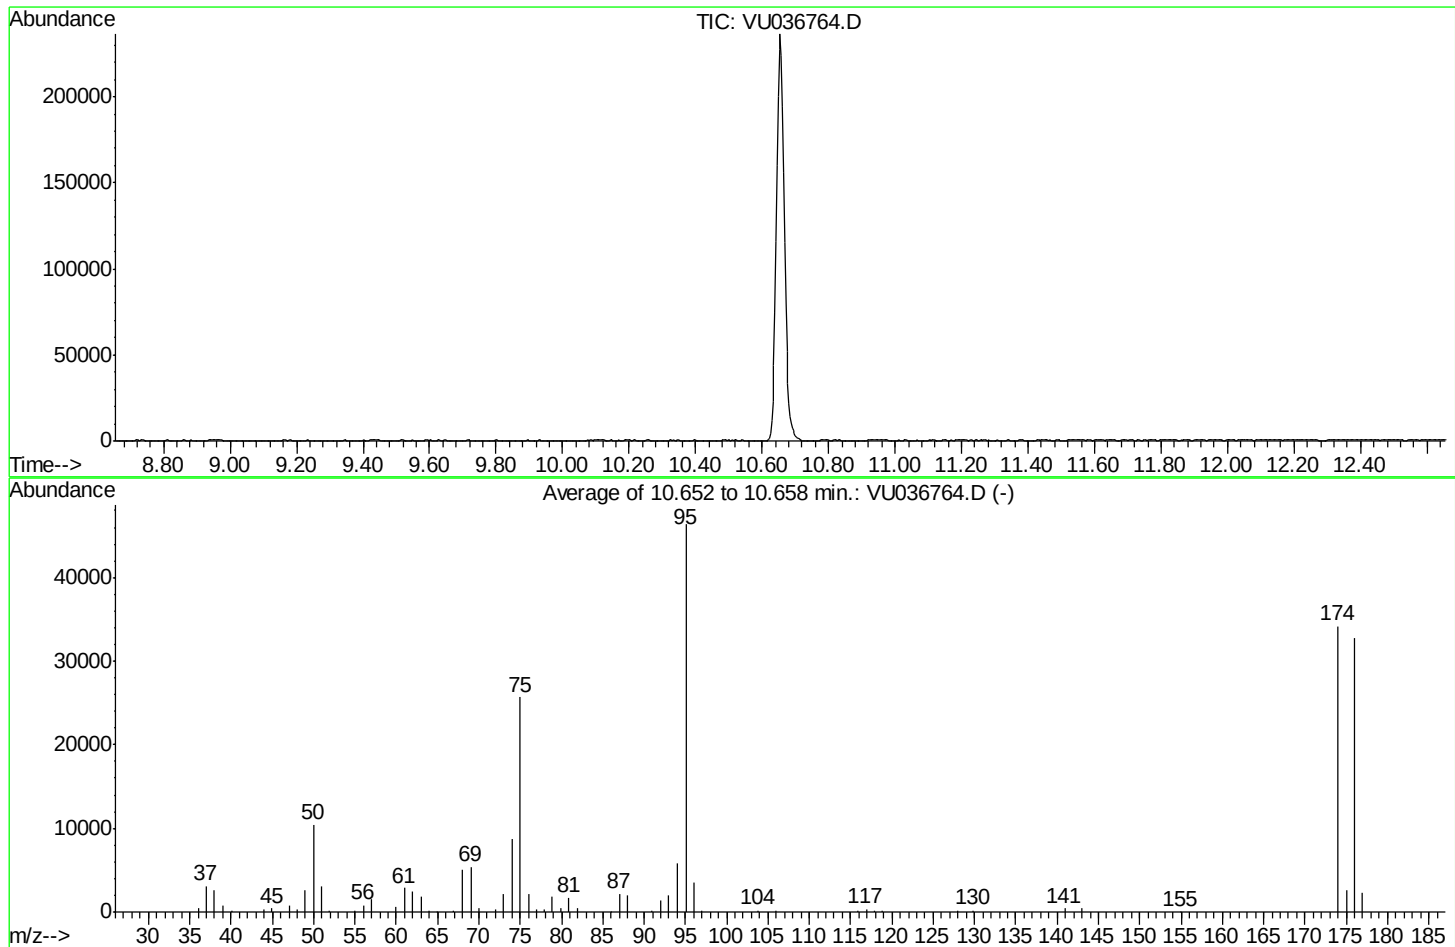

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	10433	PASS
75	95	30	80	55.4	25701	PASS
95	95	100	100	100.0	46357	PASS
96	95	5	9	7.6	3520	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	34136	PASS
175	174	5	9	7.6	2595	PASS
176	174	95	101	96.1	32794	PASS
177	176	5	9	6.8	2242	PASS

m/z	Abundance
36.00	486.0
37.00	3224.0
38.00	2582.0
39.00	906.0
40.00	120.0
43.90	604.0
44.90	442.0
47.00	762.0
48.00	382.0
49.00	2566.0
50.00	10529.0
51.00	3085.0
52.10	133.0
54.90	182.0
56.00	900.0
57.00	1509.0
60.00	667.0
61.00	2902.0
62.00	2491.0
63.00	1814.0
64.00	236.0
66.90	161.0
68.00	4998.0
69.00	5487.0
70.00	444.0
72.00	302.0
73.00	2214.0
74.10	8538.0
75.00	26080.0
76.00	2157.0
77.00	320.0
77.90	273.0
78.90	1768.0
79.90	511.0
80.90	1804.0
81.90	421.0
87.00	2285.0
88.00	2196.0
90.90	206.0
92.00	1322.0
93.00	2105.0
94.00	5997.0
95.10	45320.0
96.00	3497.0
103.80	228.0
105.90	195.0
115.80	138.0
116.90	333.0
117.90	187.0
118.90	235.0
127.90	147.0
129.90	190.0
140.90	415.0
143.00	443.0
154.90	122.0
174.00	33240.0
175.00	2526.0
176.00	32072.0
177.00	2216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	540.0
37.00	3230.0
38.00	2688.0
39.10	859.0
40.10	146.0
43.90	571.0
44.90	411.0
47.00	743.0
48.00	394.0
49.00	2693.0
50.00	10737.0
51.00	3071.0
51.90	139.0
54.90	157.0
56.00	826.0
57.00	1594.0
60.00	589.0
61.00	2966.0
62.00	2519.0
63.00	1905.0
64.00	220.0
64.90	100.0
66.90	161.0
68.00	5166.0
69.00	5515.0
70.00	451.0
72.00	355.0
73.00	2252.0
74.00	8963.0
75.00	26392.0
76.00	2114.0
77.00	342.0
77.80	301.0
78.90	1842.0
79.90	523.0
80.90	1765.0
81.90	479.0
87.00	2246.0
88.00	2129.0
90.90	188.0
92.00	1421.0
93.00	2165.0
94.00	6103.0
95.10	47856.0
96.00	3650.0
97.00	140.0
103.80	248.0
106.00	188.0
115.80	159.0
116.90	367.0
117.90	192.0
118.90	205.0
127.90	153.0
129.80	189.0
140.90	447.0
143.00	405.0
155.00	111.0
174.00	35256.0
175.00	2652.0
176.00	33904.0
177.00	2352.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	538.0
37.00	2894.0
38.00	2537.0
39.10	768.0
40.00	133.0
43.90	550.0
45.00	410.0
47.00	621.0
48.00	352.0
49.00	2492.0
50.00	10033.0
51.00	2896.0
51.90	148.0
54.90	130.0
56.00	733.0
57.00	1529.0
60.00	452.0
61.00	2688.0
62.00	2413.0
63.00	1918.0
64.00	162.0
64.90	110.0
66.90	149.0
68.00	4918.0
69.00	5249.0
70.00	424.0
72.00	359.0
73.00	2164.0
74.00	8654.0
75.00	24632.0
76.00	1960.0
77.00	288.0
77.80	275.0
78.90	1745.0
79.90	541.0
80.90	1617.0
82.00	468.0
86.00	104.0
87.00	2021.0
88.00	1875.0
91.00	157.0
92.00	1370.0
93.00	1936.0
94.00	5578.0
95.10	45896.0
96.00	3414.0
97.00	146.0
103.80	217.0
106.00	170.0
115.90	160.0
116.90	332.0
117.90	171.0
118.80	153.0
127.90	161.0
129.80	177.0
140.90	432.0
143.00	339.0
174.00	33912.0
175.00	2609.0
176.00	32408.0
177.00	2160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
43.90	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06