

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
 Data File : VU053080.D
 Acq On : 13 Feb 2023 14:58
 Operator : JC/MD
 Sample : 01533-07DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM78DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	37	52	73	rBV	857904	1083376	100.00%	23.840%
2	1.598	150	158	168	rBV	32319	38139	3.52%	0.839%
3	1.913	248	256	266	rBV	33887	45505	4.20%	1.001%
4	2.566	447	459	473	rVB2	59830	100499	9.28%	2.212%
5	3.180	635	650	667	rVB2	7181	15857	1.46%	0.349%
6	4.640	1087	1104	1137	rBV4	58920	228270	21.07%	5.023%
7	5.058	1217	1234	1253	rBV2	66255	145112	13.39%	3.193%
8	5.720	1419	1440	1459	rBV3	118235	310379	28.65%	6.830%
9	6.244	1590	1603	1621	rBV	141521	266897	24.64%	5.873%
10	6.537	1681	1694	1713	rBV	243124	454212	41.93%	9.995%
11	6.685	1724	1740	1755	rBV	80628	156052	14.40%	3.434%
12	7.559	1999	2012	2029	rBV	43213	75256	6.95%	1.656%
13	7.894	2100	2116	2131	rBV	144443	247588	22.85%	5.448%
14	8.177	2192	2204	2219	rBV2	26213	44309	4.09%	0.975%
15	8.630	2333	2345	2378	rBV2	210251	400578	36.97%	8.815%
16	9.411	2576	2588	2606	rBV	186590	306941	28.33%	6.754%
17	10.752	2994	3005	3020	rBV	68444	107501	9.92%	2.366%
18	11.807	3321	3333	3354	rVB	183962	288674	26.65%	6.352%
19	12.189	3441	3452	3470	rBV	143524	229153	21.15%	5.043%




Sum of corrected areas: 4544298

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053080.D
Acq On : 13 Feb 2023 14:58
Operator : JC/MD
Sample : 01533-07DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M78DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

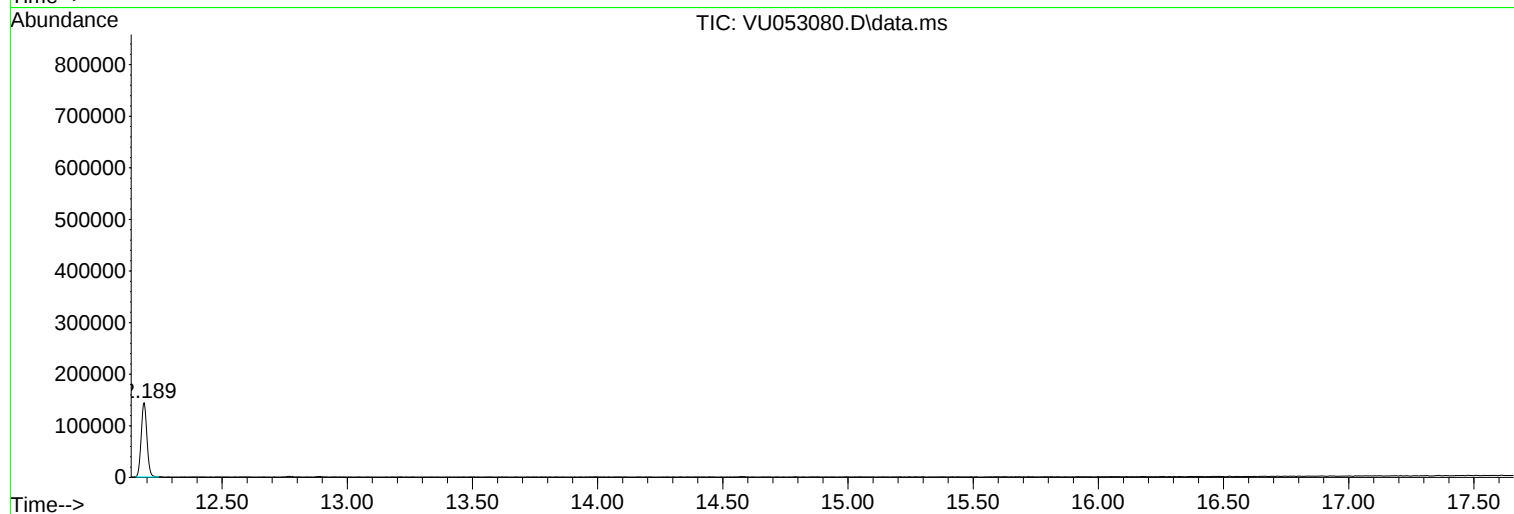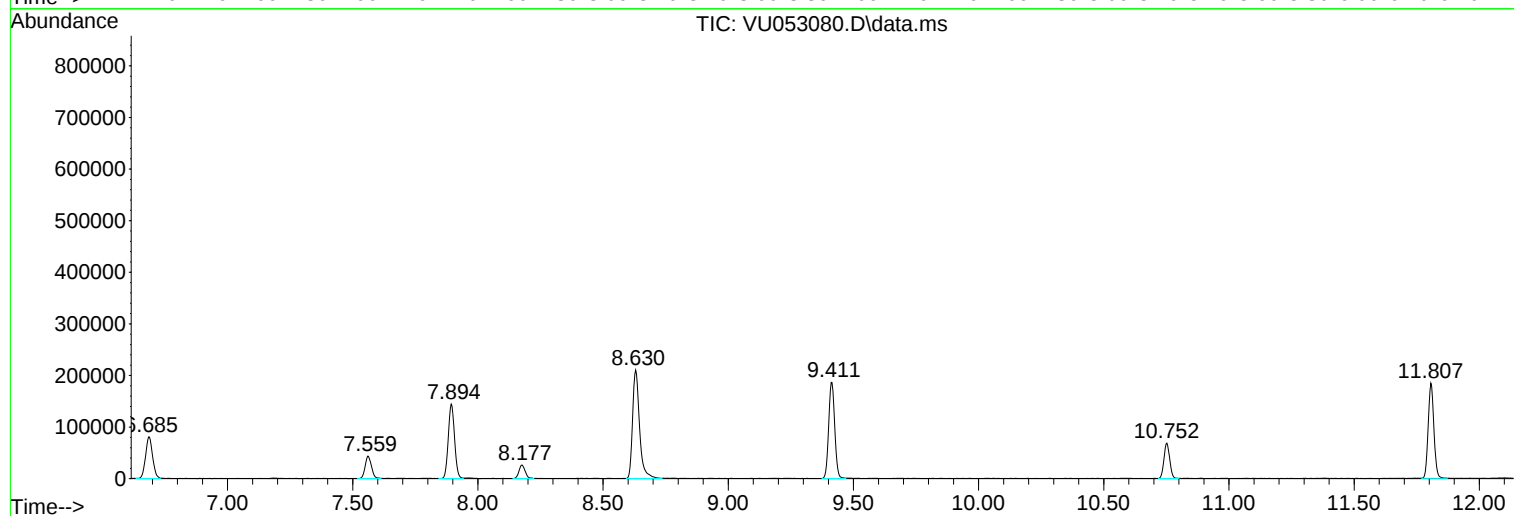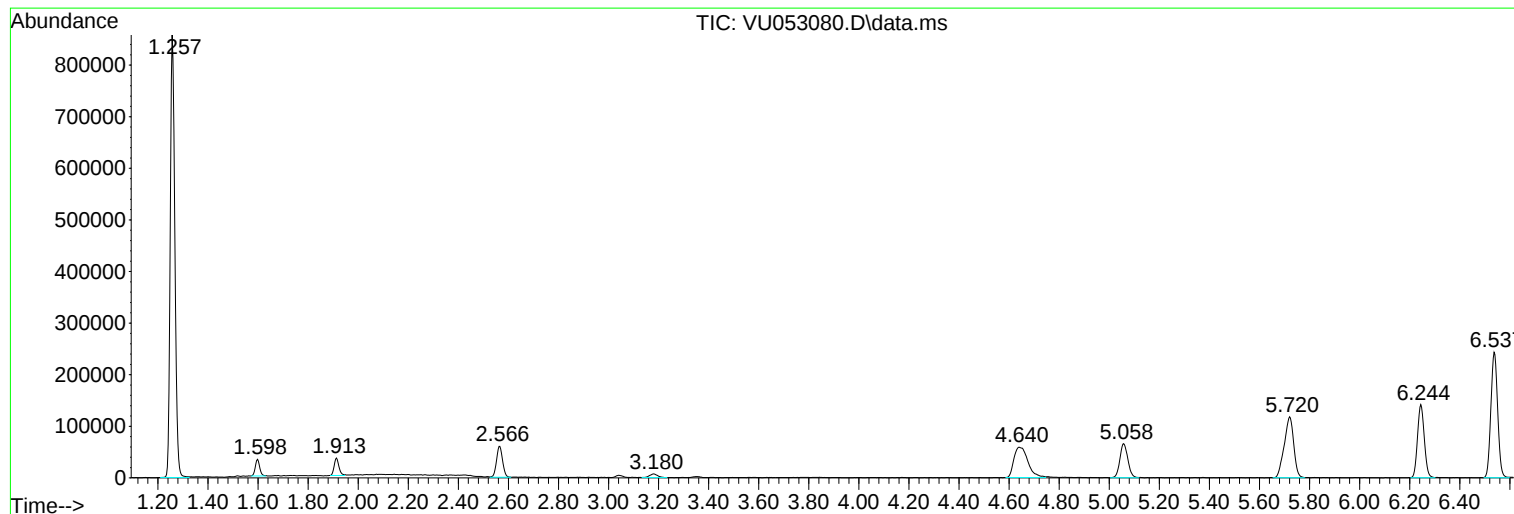

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053080.D
Acq On : 13 Feb 2023 14:58
Operator : JC/MD
Sample : 01533-07DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM78DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053080.D
Acq On : 13 Feb 2023 14:58
Operator : JC/MD
Sample : 01533-07DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM78DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc