

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
 Data File : VU053082.D
 Acq On : 13 Feb 2023 15:47
 Operator : JC/MD
 Sample : 01533-03DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM19DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	35	52	73	rBV	962507	1257833	100.00%	27.999%
2	1.598	150	158	167	rBV	29658	33931	2.70%	0.755%
3	1.913	246	256	270	rBV	31139	43998	3.50%	0.979%
4	2.563	448	458	474	rVB	54839	91199	7.25%	2.030%
5	3.183	638	651	665	rVB	7090	15602	1.24%	0.347%
6	4.653	1088	1108	1144	rBV3	56922	227815	18.11%	5.071%
7	5.058	1219	1234	1251	rBV2	61710	136079	10.82%	3.029%
8	5.720	1419	1440	1463	rBV2	110985	292691	23.27%	6.515%
9	6.244	1590	1603	1621	rBV	141032	269243	21.41%	5.993%
10	6.537	1680	1694	1714	rBV2	168231	313944	24.96%	6.988%
11	6.685	1725	1740	1758	rBV2	75871	149265	11.87%	3.323%
12	7.563	2002	2013	2030	rBV2	40097	69401	5.52%	1.545%
13	7.894	2104	2116	2134	rBV	132979	227004	18.05%	5.053%
14	8.177	2194	2204	2219	rBV	24221	40722	3.24%	0.906%
15	8.630	2332	2345	2375	rBV2	207691	400239	31.82%	8.909%
16	9.411	2576	2588	2612	rBV	185961	308397	24.52%	6.865%
17	10.752	2993	3005	3019	rVB	66617	104448	8.30%	2.325%
18	11.807	3322	3333	3352	rBV	185451	294380	23.40%	6.553%
19	12.189	3439	3452	3467	rBV	131653	216188	17.19%	4.812%




Sum of corrected areas: 4492379

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053082.D
Acq On : 13 Feb 2023 15:47
Operator : JC/MD
Sample : 01533-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM19DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

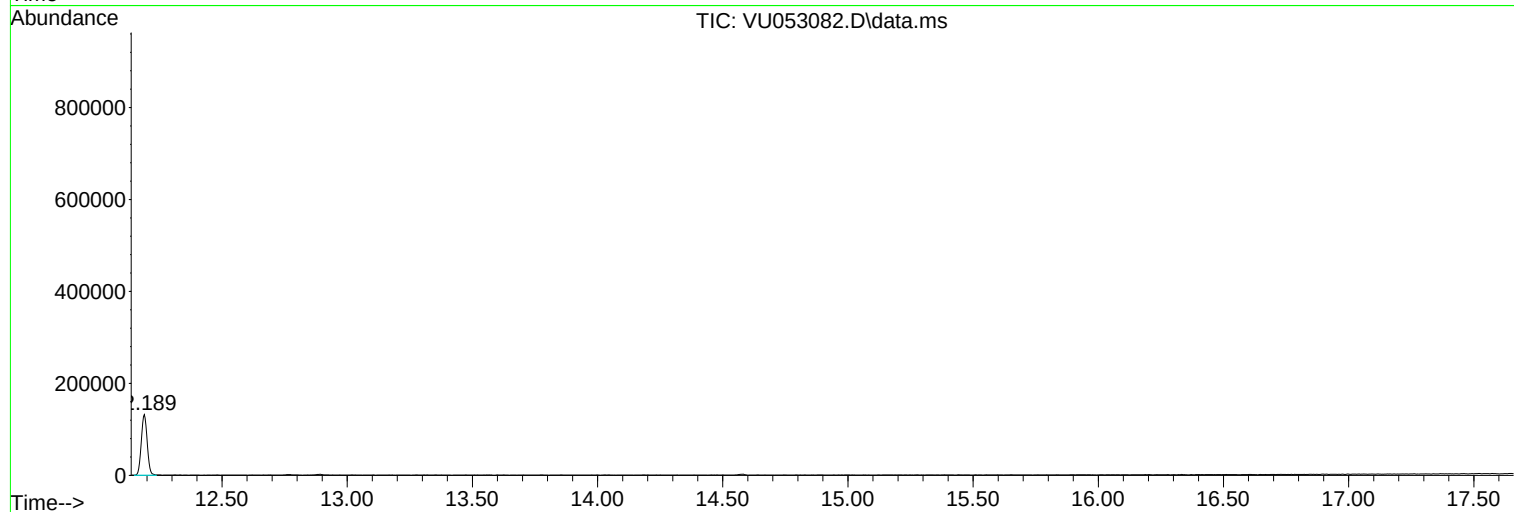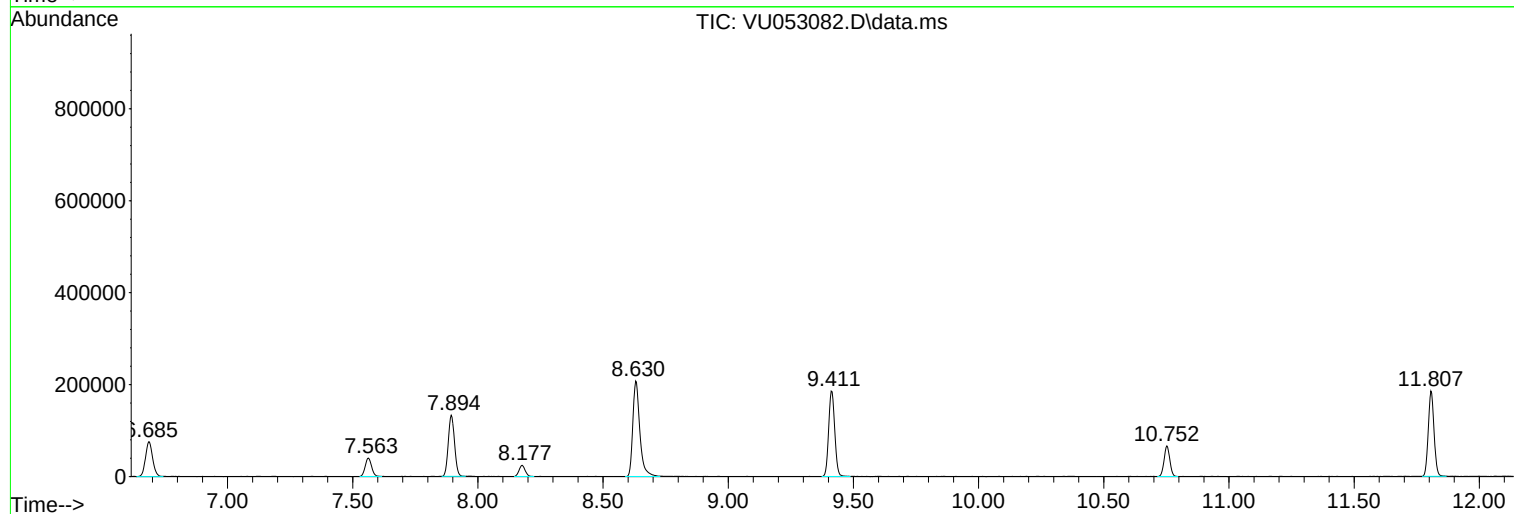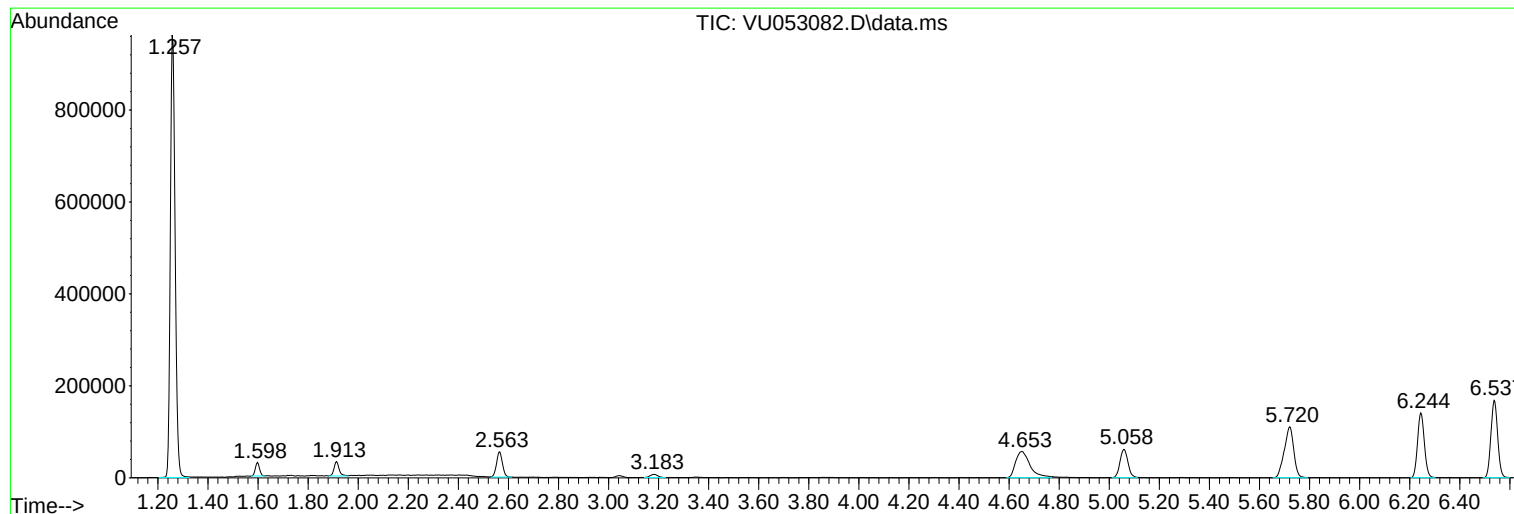

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053082.D
Acq On : 13 Feb 2023 15:47
Operator : JC/MD
Sample : 01533-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M19DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053082.D
Acq On : 13 Feb 2023 15:47
Operator : JC/MD
Sample : 01533-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M19DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------