

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
 Data File : VU053084.D
 Acq On : 13 Feb 2023 16:36
 Operator : JC/MD
 Sample : 01533-05DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM76DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	40	52	71	rBV	996558	1312206	100.00%	27.362%
2	1.598	151	158	167	rVB	30784	35000	2.67%	0.730%
3	1.913	246	256	266	rBV	30690	44070	3.36%	0.919%
4	2.563	445	458	480	rVB2	56360	97434	7.43%	2.032%
5	3.180	634	650	665	rVB2	7901	17886	1.36%	0.373%
6	4.653	1085	1108	1143	rBV4	64591	245133	18.68%	5.111%
7	5.058	1218	1234	1257	rBV	62292	137528	10.48%	2.868%
8	5.720	1420	1440	1463	rBV3	112731	296752	22.61%	6.188%
9	6.244	1590	1603	1621	rBV	143829	267895	20.42%	5.586%
10	6.537	1681	1694	1717	rBV	286446	531570	40.51%	11.084%
11	6.685	1728	1740	1757	rBV	75930	147429	11.24%	3.074%
12	7.563	2000	2013	2033	rVB2	40469	71205	5.43%	1.485%
13	7.894	2104	2116	2134	rBV	135085	231836	17.67%	4.834%
14	8.177	2193	2204	2220	rBV2	24994	42402	3.23%	0.884%
15	8.630	2333	2345	2372	rBV2	207365	395146	30.11%	8.239%
16	9.411	2573	2588	2609	rBV	185826	307453	23.43%	6.411%
17	10.752	2993	3005	3022	rVB	64018	103525	7.89%	2.159%
18	11.807	3320	3333	3348	rBV	184950	291846	22.24%	6.085%
19	12.189	3437	3452	3466	rBV	135595	219478	16.73%	4.576%




Sum of corrected areas: 4795794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053084.D
Acq On : 13 Feb 2023 16:36
Operator : JC/MD
Sample : 01533-05DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

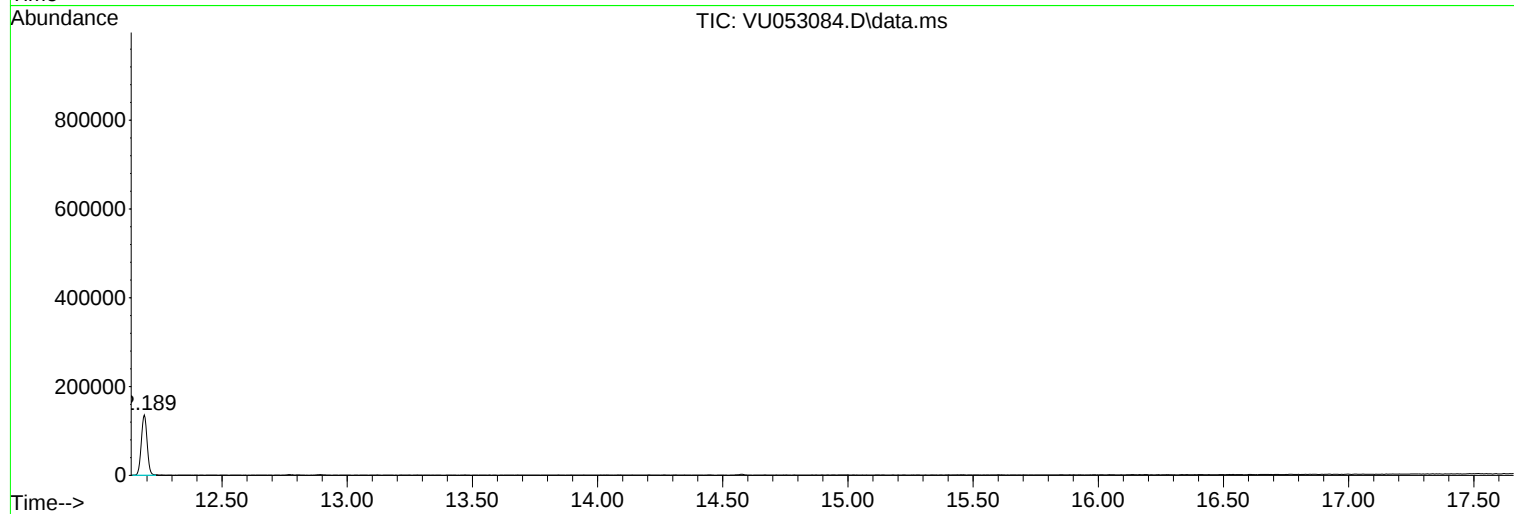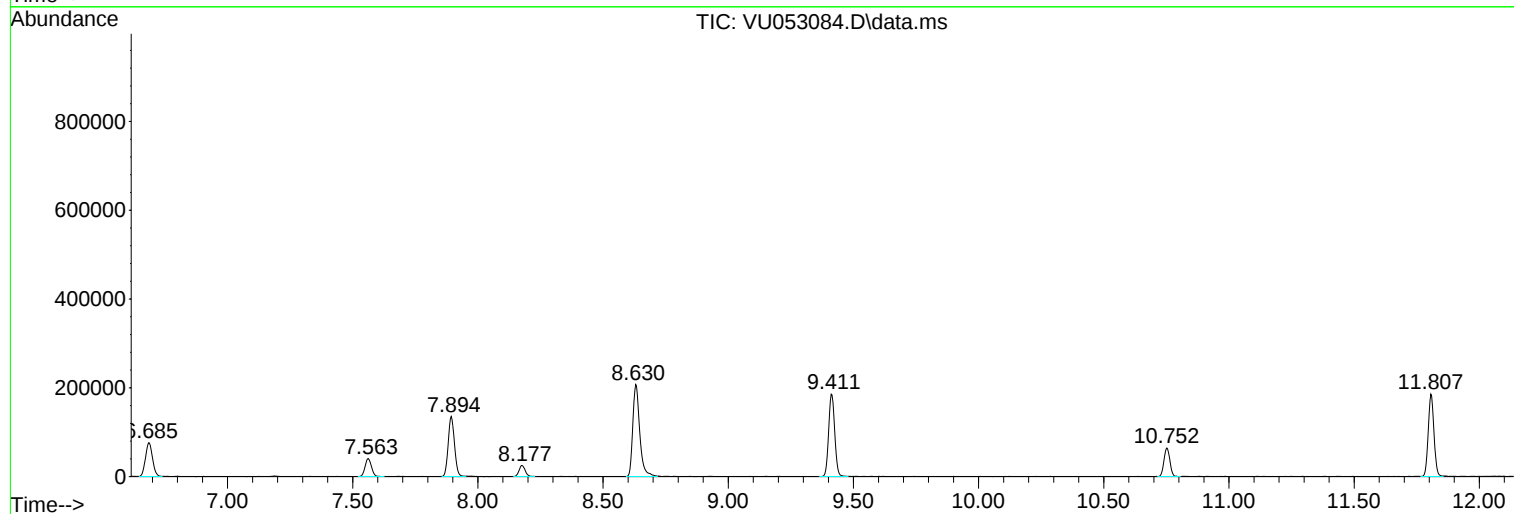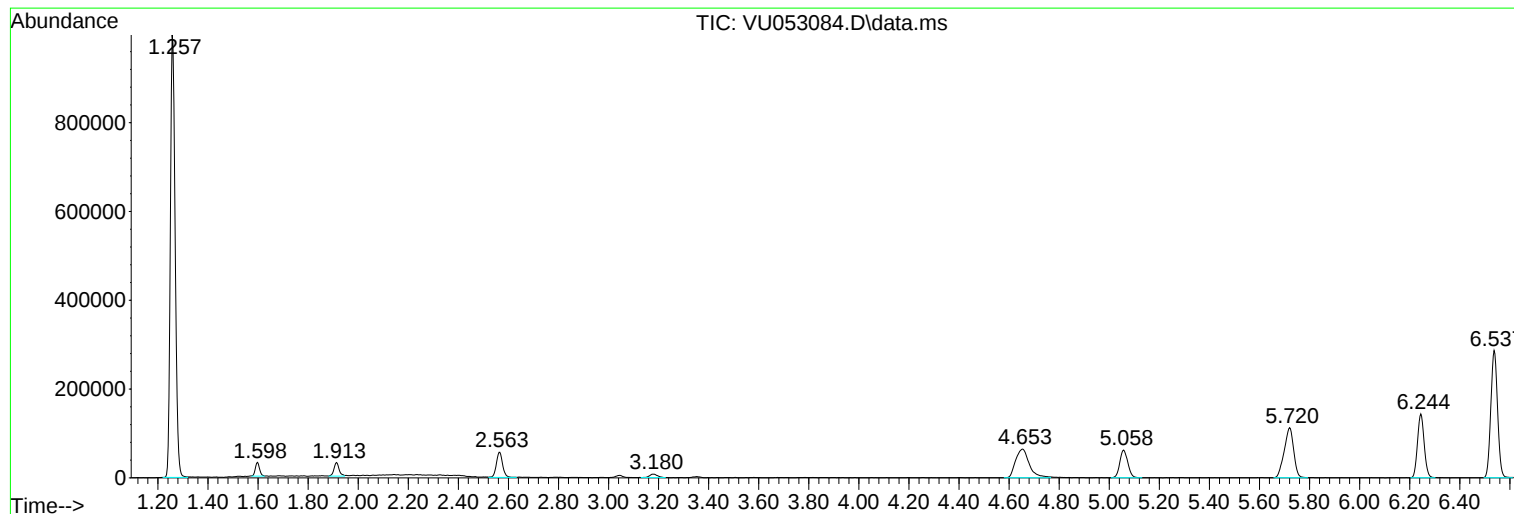

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053084.D
Acq On : 13 Feb 2023 16:36
Operator : JC/MD
Sample : 01533-05DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053084.D
Acq On : 13 Feb 2023 16:36
Operator : JC/MD
Sample : 01533-05DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc