

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
 Data File : VU053085.D
 Acq On : 13 Feb 2023 17:00
 Operator : JC/MD
 Sample : 01533-06DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM77DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	39	52	69	rBV	1007598	1319509	100.00%	28.580%
2	1.598	151	158	170	rVB	30558	34931	2.65%	0.757%
3	1.913	247	256	269	rBV	32602	44284	3.36%	0.959%
4	2.566	447	459	472	rVB2	57037	94744	7.18%	2.052%
5	3.180	636	650	665	rBV	6227	14230	1.08%	0.308%
6	4.643	1089	1105	1145	rBV3	57617	221475	16.78%	4.797%
7	5.058	1218	1234	1251	rBV	65463	142444	10.80%	3.085%
8	5.720	1420	1440	1462	rBV2	115021	303268	22.98%	6.569%
9	6.244	1588	1603	1629	rBV	136954	263055	19.94%	5.698%
10	6.537	1676	1694	1713	rBV	187410	349514	26.49%	7.570%
11	6.685	1726	1740	1757	rBV	79454	154350	11.70%	3.343%
12	7.563	2000	2013	2027	rBV2	40507	71242	5.40%	1.543%
13	7.894	2104	2116	2135	rBV	137518	238426	18.07%	5.164%
14	8.177	2193	2204	2216	rBV2	24961	41868	3.17%	0.907%
15	8.630	2332	2345	2374	rBV2	212162	404998	30.69%	8.772%
16	9.415	2575	2589	2605	rBV	179458	302962	22.96%	6.562%
17	10.752	2994	3005	3019	rBV	65552	105782	8.02%	2.291%
18	11.807	3320	3333	3350	rBV	180253	287391	21.78%	6.225%
19	12.189	3439	3452	3476	rVB	136560	222358	16.85%	4.816%




Sum of corrected areas: 4616831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053085.D
Acq On : 13 Feb 2023 17:00
Operator : JC/MD
Sample : 01533-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M77DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

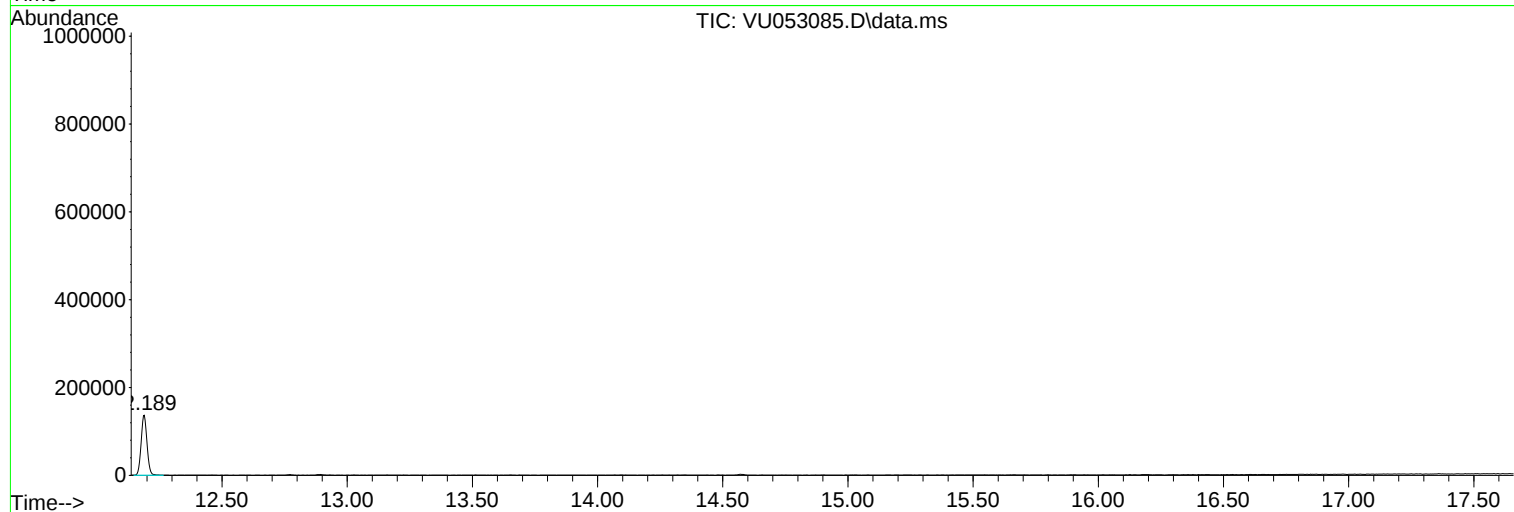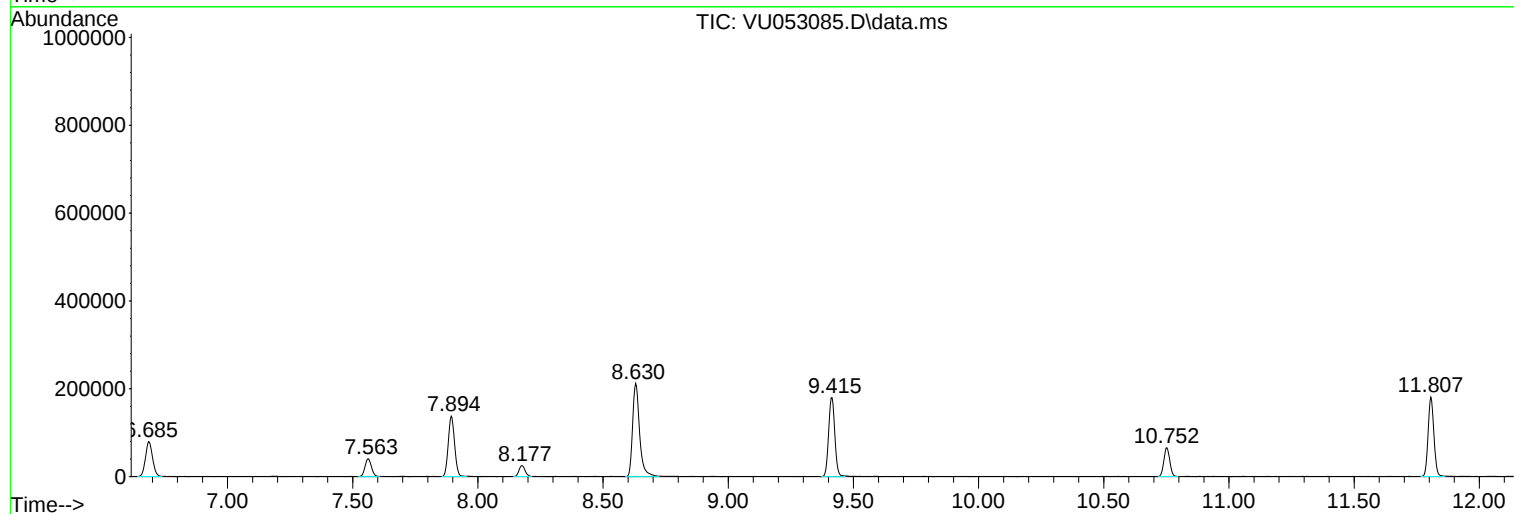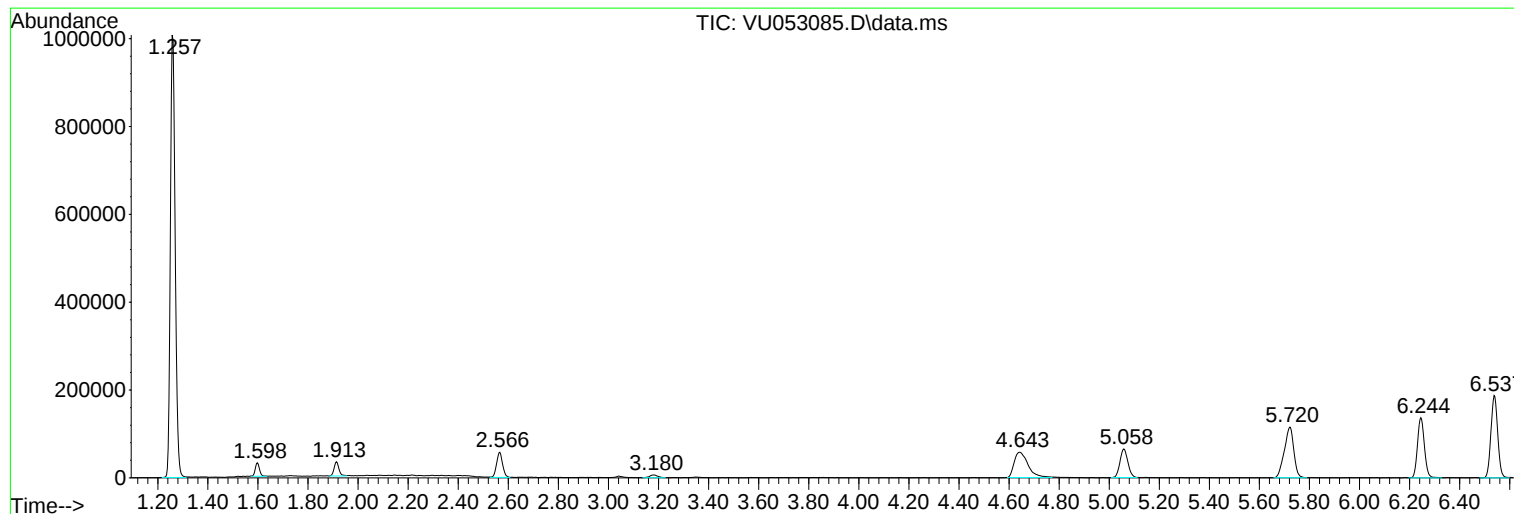

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053085.D
Acq On : 13 Feb 2023 17:00
Operator : JC/MD
Sample : 01533-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM77DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053085.D
Acq On : 13 Feb 2023 17:00
Operator : JC/MD
Sample : 01533-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M77DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc