
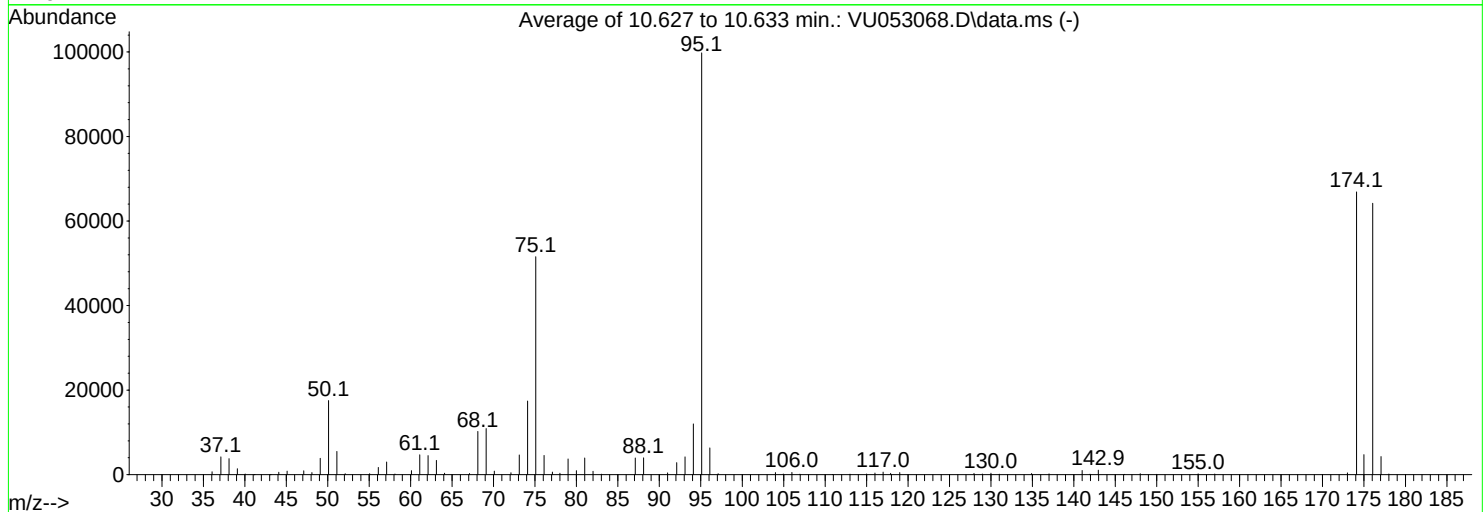


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021323\
Data File : VU053068.D
Acq On : 13 Feb 2023 09:34
Operator : JC/MD
Sample : BFB197
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB197

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Feb 14 00:41:52 2023

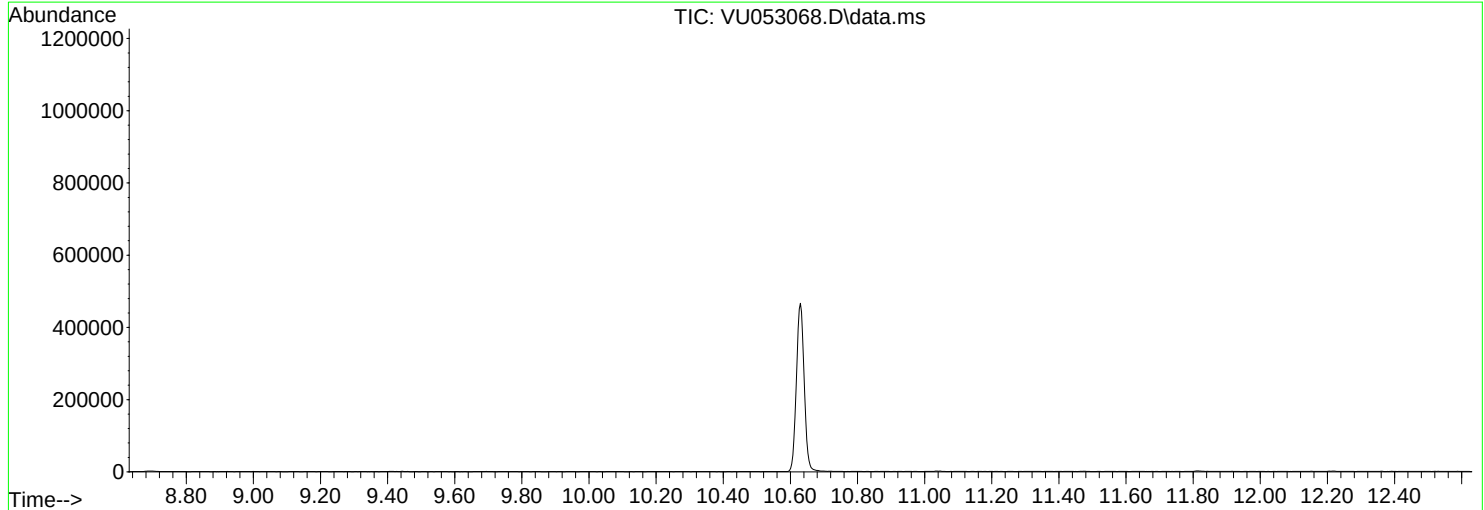

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2953

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	17517	PASS
75	95	30	80	51.7	51552	PASS
95	95	100	100	100.0	99792	PASS
96	95	5	9	6.4	6342	PASS
173	174	0.00	2	0.6	405	PASS
174	95	50	120	67.0	66909	PASS
175	174	5	9	7.1	4739	PASS
176	174	95	101	96.0	64213	PASS
177	176	5	9	6.7	4287	PASS

m/z	Abundance
36.00	173.0
41.10	142.0
43.00	141.0
44.10	200.0
55.10	170.0
71.00	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197

m/z	Abundance
36.10	881.0
37.10	4241.0
38.10	3929.0
39.10	1399.0
40.00	185.0
41.10	140.0
43.20	161.0
44.10	739.0
45.10	804.0
47.10	966.0
48.10	522.0
49.10	3937.0
50.10	18192.0
51.10	5438.0
52.10	246.0
55.10	441.0
56.10	1768.0
57.10	2985.0
58.00	148.0
60.10	889.0
61.10	4660.0
62.10	4589.0
63.10	3336.0
64.10	332.0
67.10	251.0
68.10	10329.0
69.10	11013.0
70.10	831.0
71.10	113.0
72.10	471.0
73.10	4689.0
74.10	17608.0
75.10	51320.0
76.10	4653.0
77.10	616.0
78.00	339.0
79.00	3829.0
80.00	954.0
81.00	3965.0
82.00	746.0
83.10	134.0
87.10	3686.0
88.10	4024.0
91.00	404.0
92.10	2776.0
93.10	4166.0
94.10	11971.0
95.10	99112.0
96.10	6408.0
97.10	250.0
104.00	477.0
105.00	183.0
106.00	582.0
106.90	108.0
110.90	118.0
113.00	102.0
115.00	144.0
116.00	399.0
117.00	708.0
117.90	310.0
119.00	591.0
128.00	264.0
129.00	170.0
130.00	316.0
131.00	125.0
134.90	288.0
137.00	185.0
141.00	1025.0
142.00	118.0
143.00	1038.0
146.10	119.0
148.00	206.0
155.00	198.0
157.00	154.0
173.10	395.0
174.10	65368.0
175.00	4632.0
176.10	62632.0
177.00	4191.0
178.00	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197

m/z	Abundance
36.10	846.0
37.10	4343.0
38.10	3903.0
39.10	1399.0
40.00	165.0
41.10	157.0
43.20	167.0
44.10	785.0
45.10	842.0
47.10	906.0
48.10	499.0
49.10	3980.0
50.10	17968.0
51.10	5658.0
52.10	230.0
55.00	445.0
56.10	1786.0
57.10	3087.0
58.10	142.0
60.10	1002.0
61.10	4842.0
62.10	4694.0
63.10	3472.0
64.10	350.0
67.10	271.0
68.10	10485.0
69.10	11186.0
70.10	882.0
72.10	460.0
73.10	4784.0
74.10	17936.0
75.10	53184.0
76.10	4642.0
77.10	619.0
78.00	358.0
79.00	3832.0
80.00	974.0
81.00	4026.0
82.00	794.0
83.10	118.0
87.10	3999.0
88.10	4121.0
91.00	452.0
92.10	2966.0
93.10	4322.0
94.10	12324.0
95.10	103056.0
96.10	6479.0
97.10	233.0
104.00	510.0
104.90	156.0
106.00	545.0
107.00	132.0
113.00	118.0
115.00	154.0
116.00	410.0
117.00	628.0
117.90	319.0
119.00	499.0
128.00	299.0
129.00	162.0
130.00	367.0
131.00	116.0
134.90	301.0
137.00	189.0
141.00	1007.0
141.90	118.0
143.00	1090.0
146.10	109.0
148.00	221.0
150.00	109.0
155.00	209.0
157.00	150.0
173.00	422.0
174.10	68888.0
175.00	4912.0
176.00	66168.0
177.00	4411.0
178.00	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197

m/z	Abundance
36.10	789.0
37.10	4078.0
38.10	3537.0
39.10	1358.0
40.10	145.0
41.10	159.0
43.10	161.0
44.10	749.0
45.10	830.0
47.10	807.0
48.10	446.0
49.10	3716.0
50.10	16392.0
51.10	5438.0
52.10	226.0
55.00	366.0
56.10	1590.0
57.10	2915.0
58.20	123.0
60.10	980.0
61.10	4543.0
62.10	4288.0
63.10	3344.0
64.10	331.0
67.10	275.0
68.10	9797.0
69.10	10484.0
70.10	839.0
72.10	457.0
73.10	4494.0
74.10	16736.0
75.10	50152.0
76.10	4311.0
77.10	531.0
78.00	343.0
79.00	3494.0
80.00	934.0
81.00	3769.0
82.00	822.0
83.00	100.0
87.10	4146.0
88.10	3816.0
91.00	449.0
92.10	2812.0
93.10	4129.0
94.10	11728.0
95.10	97208.0
96.10	6138.0
97.10	194.0
104.00	513.0
104.90	149.0
106.00	497.0
107.00	151.0
113.00	127.0
115.00	120.0
116.00	381.0
117.00	533.0
117.90	314.0
119.00	395.0
127.90	302.0
128.90	165.0
130.00	353.0
131.00	106.0
134.90	223.0
137.00	159.0
141.00	947.0
141.90	108.0
142.90	1037.0
148.00	228.0
150.00	109.0
155.00	204.0
157.00	139.0
172.90	397.0
174.10	66472.0
175.00	4674.0
176.10	63840.0
177.10	4259.0
178.00	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197