

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU021419\
 Data File : VU029455.D
 Acq On : 14 Feb 2019 14:11
 Operator : JC/SP
 Sample : K1436-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESXA8

Quant Time: Feb 15 01:32:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 15 00:42:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	194279	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	181962	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	95927	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	50954	3.90	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.00%
7) Chloroethane-d5	1.68	69	50293	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.20%
11) 1,1-Dichloroethene-d2	2.27	63	91325	3.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	4.19	46	135234	49.83	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.66%
24) Chloroform-d	4.65	84	97472	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.31	65	51158	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	5.34	84	202796	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	6.33	67	62533	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.56	98	195349	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.85	79	25625	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.31	63	136665	51.40	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.80%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	52109	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	88698	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%


Target Compounds					Qvalue
13) Acetone	2.32	43	4353	1.766 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021419\
Data File : VU029455.D
Acq On : 14 Feb 2019 14:11
Operator : JC/SP
Sample : K1436-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXA8

Quant Time: Feb 15 01:32:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 15 00:42:37 2019
Response via : Initial Calibration

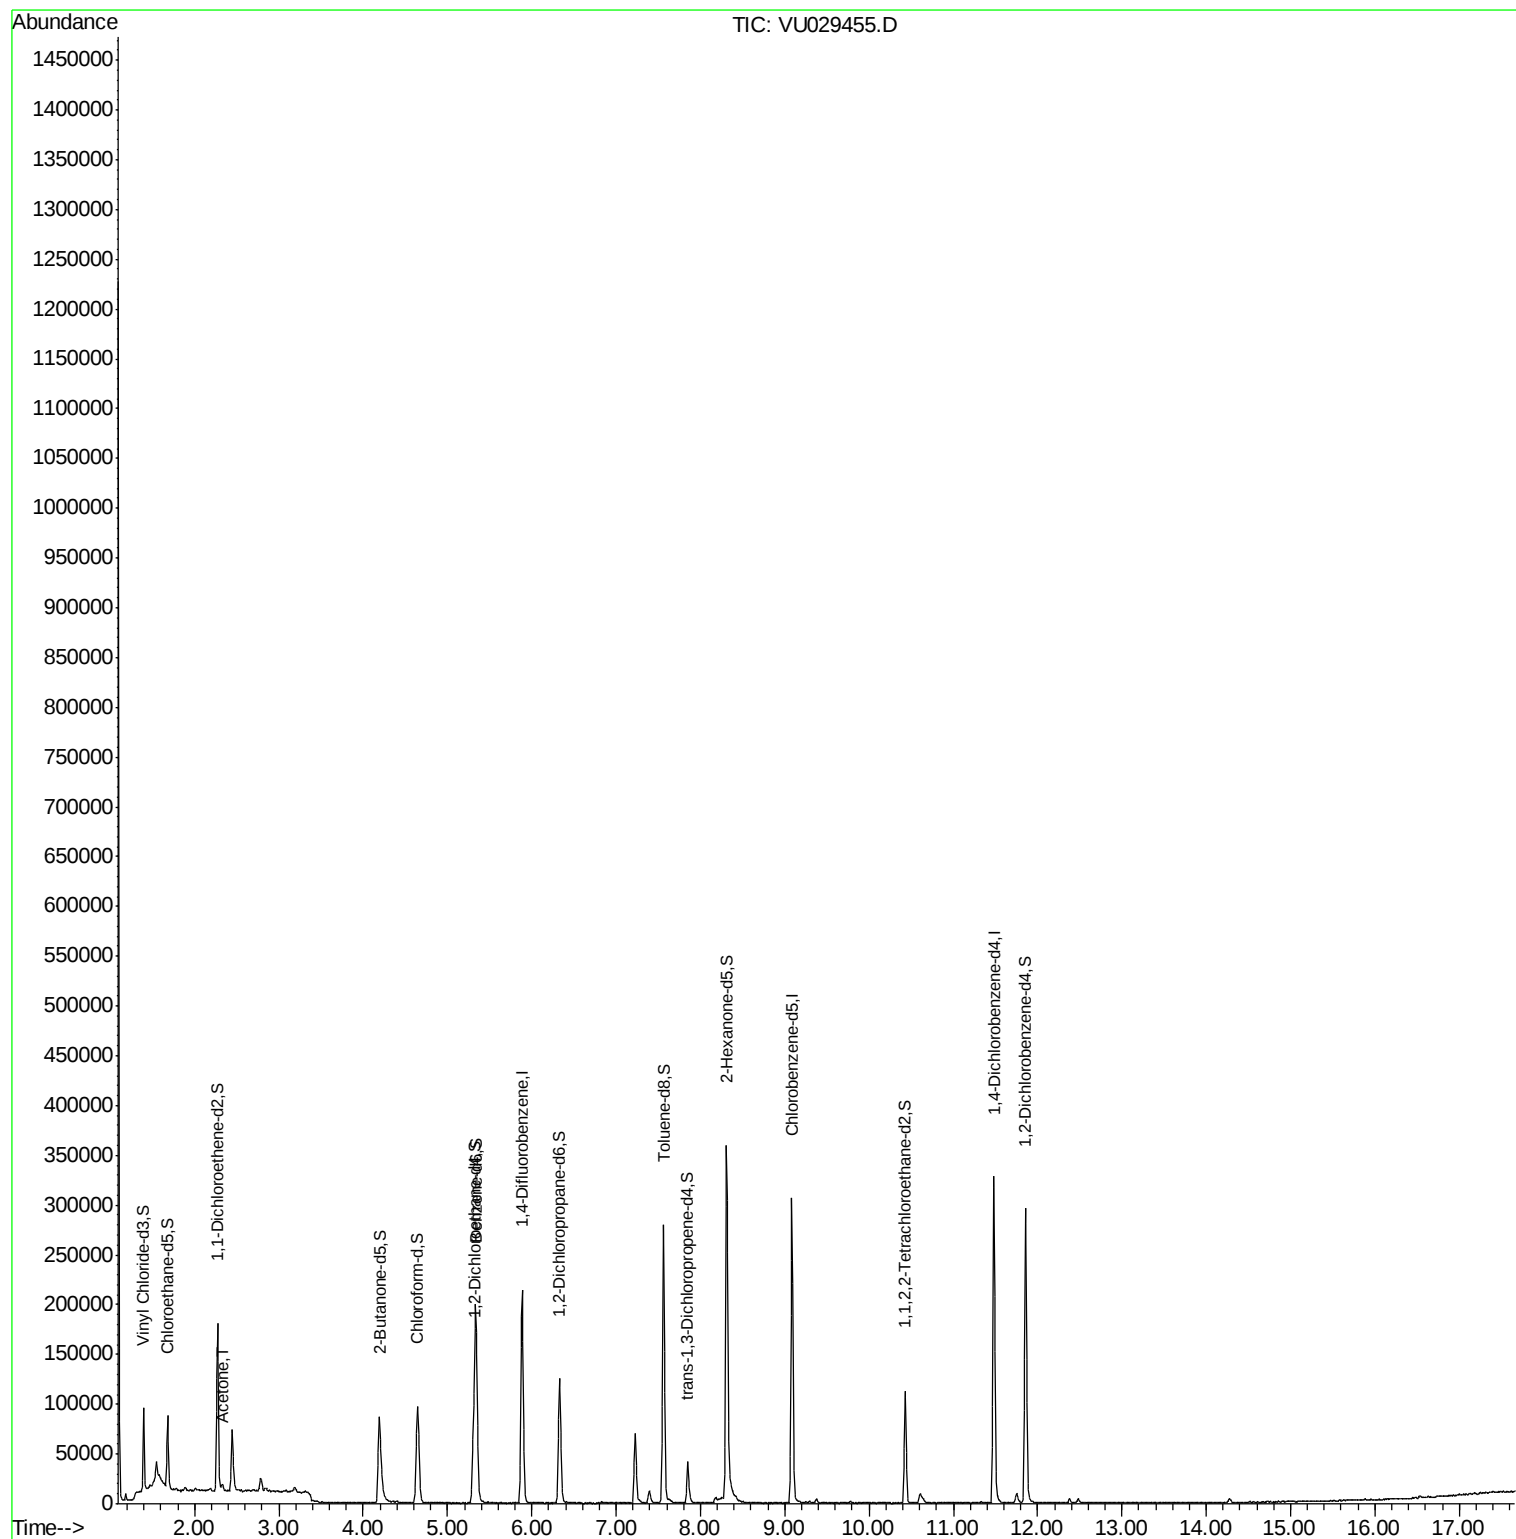

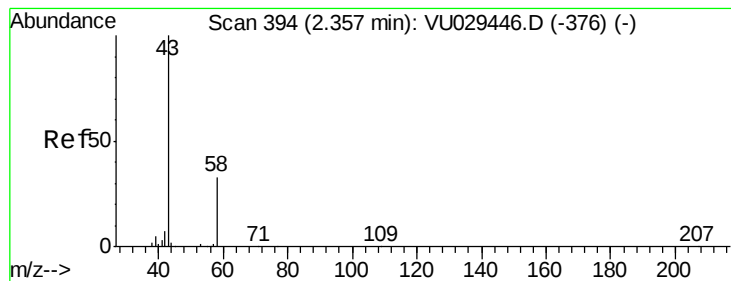

#13
 Acetone
 Concen: 1.766 ug/L
 RT: 2.32 min Scan# 384
 Delta R.T. -0.03 min
 Lab File: VU029455.D
 Acq: 14 Feb 2019 14:11

Instrument :
 MSVOA_U
 ClientSampleId :
 ESXA8

Tgt Ion: 43 Resp: 4353
 Ion Ratio Lower Upper
 43 100
 58 42.0 0.0 65.0

