

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU021419\
 Data File : VU029480.D
 Acq On : 15 Feb 2019 01:04
 Operator : JC/SP
 Sample : K1438-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESXE1

Quant Time: Feb 15 04:02:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 15 01:55:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	188003	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	176415	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	91176	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	48308	3.82	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.40%
7) Chloroethane-d5	1.68	69	48229	4.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.40%
11) 1,1-Dichloroethene-d2	2.27	63	82723	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	4.19	46	130035	49.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.02%
24) Chloroform-d	4.65	84	93611	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.31	65	48563	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
32) Benzene-d6	5.34	84	188935	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
36) 1,2-Dichloropropane-d6	6.33	67	59097	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.56	98	178319	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.20%
43) trans-1,3-Dichloropropene-	7.85	79	21760	3.89	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.80%
46) 2-Hexanone-d5	8.31	63	132253	51.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.60%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	51011	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	79450	4.72	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.40%


Target Compounds					Qvalue
13) Acetone	2.32	43	5810	2.435 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU021419\
Data File : VU029480.D
Acq On : 15 Feb 2019 01:04
Operator : JC/SP
Sample : K1438-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXE1

Quant Time: Feb 15 04:02:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 15 01:55:09 2019
Response via : Initial Calibration

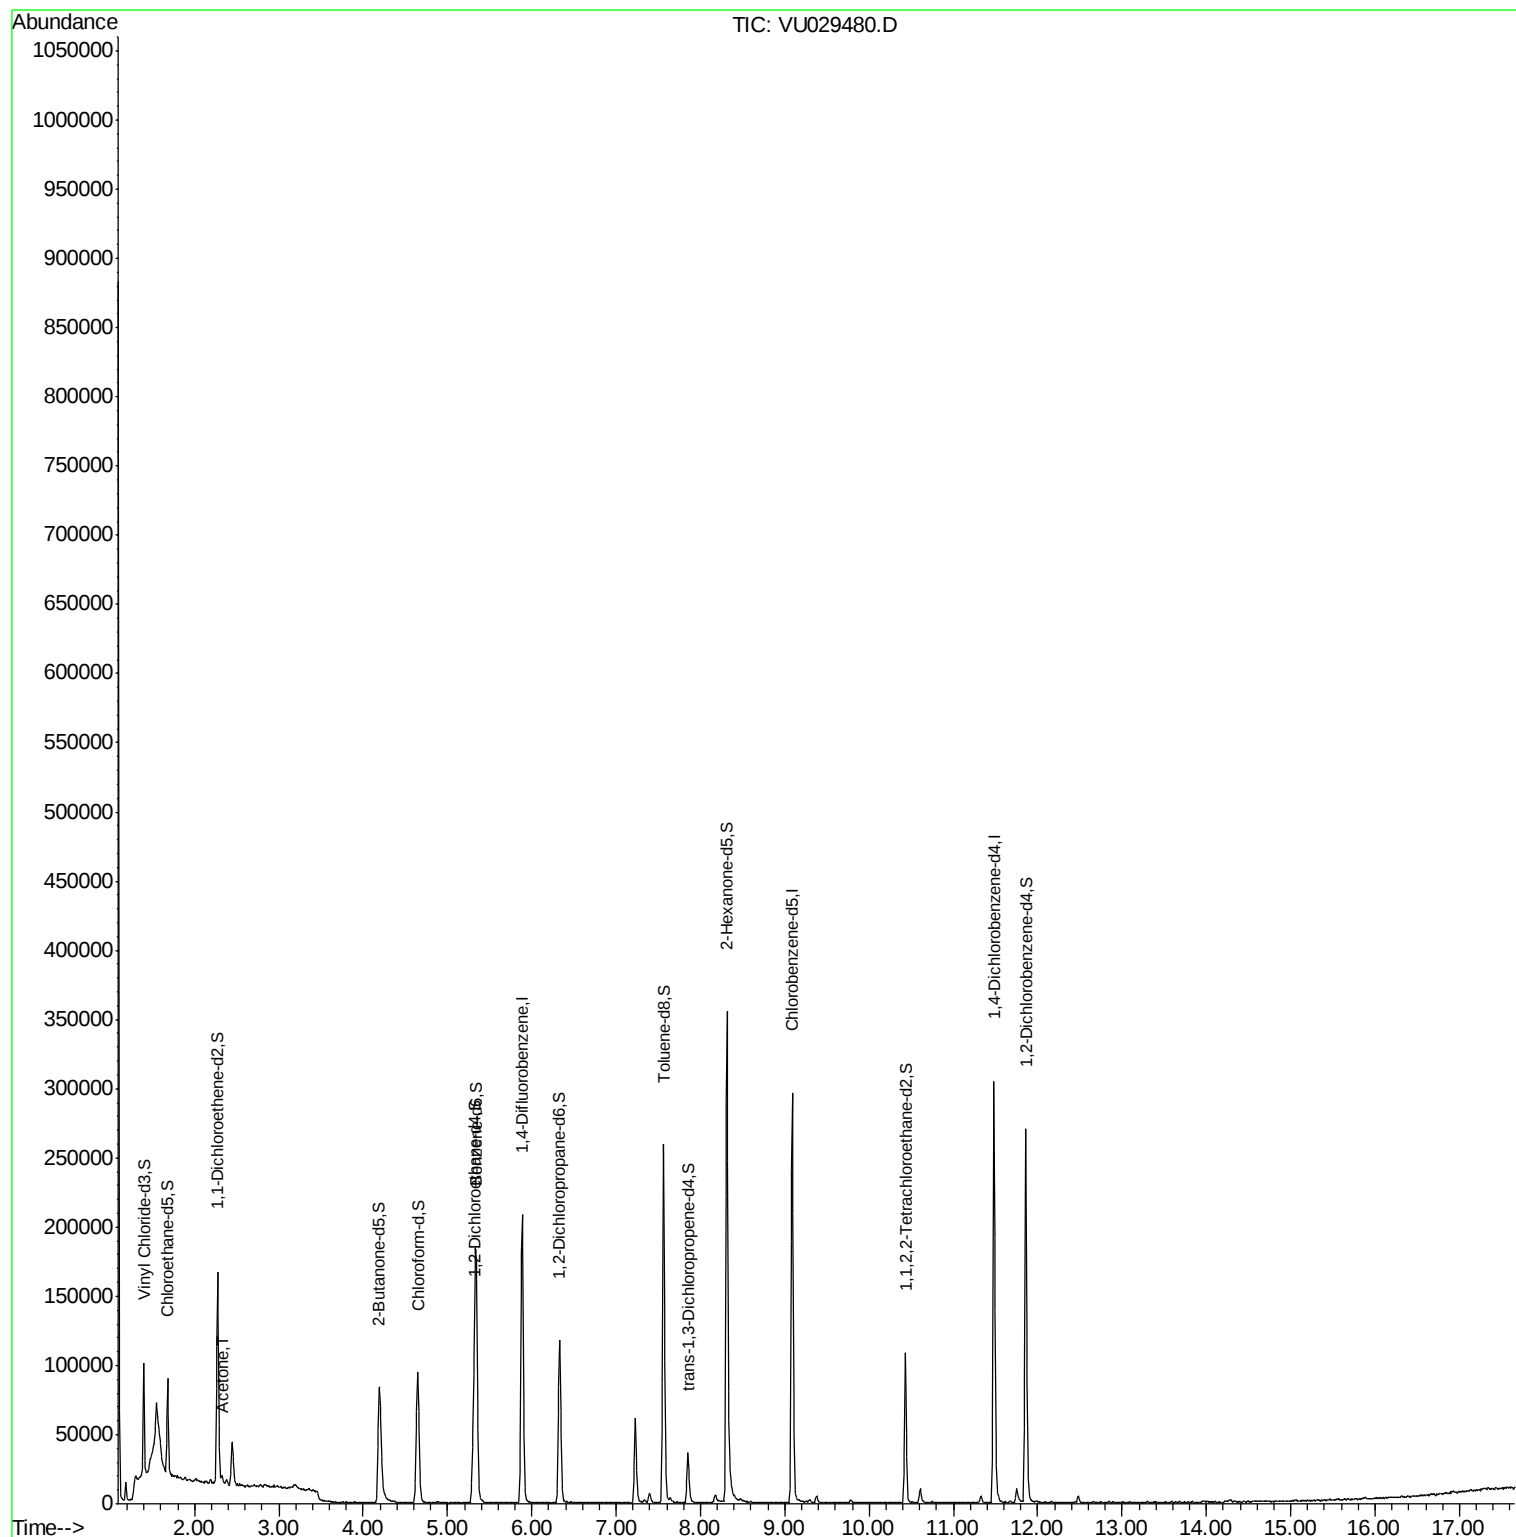

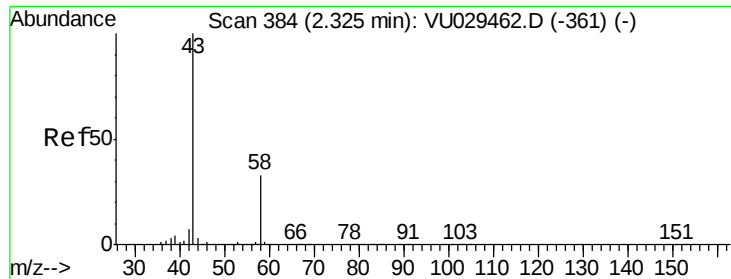

#13

Acetone

Concen: 2.435 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.00 min

Lab File: VU029480.D

Acq: 15 Feb 2019 01:04

Instrument :

MSVOA_U

ClientSampleId :

ESXE1

Tgt Ion: 43 Resp: 5810

Ion Ratio Lower Upper

43 100

58 34.6 0.0 65.0

