

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU021419\
 Data File : VU029482.D
 Acq On : 15 Feb 2019 01:51
 Operator : JC/SP
 Sample : K1438-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESXE3

Quant Time: Feb 15 04:09:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Feb 15 01:55:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	189837	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	177731	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	91427	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	47772	3.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.80%
7) Chloroethane-d5	1.68	69	49610	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.00%
11) 1,1-Dichloroethene-d2	2.27	63	84906	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	4.19	46	130226	49.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.22%
24) Chloroform-d	4.65	84	94650	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	5.31	65	51168	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.34	84	199089	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.33	67	60546	4.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.80%
41) Toluene-d8	7.56	98	184899	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	7.85	79	22985	4.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.40%
46) 2-Hexanone-d5	8.31	63	139221	53.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.20%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	53821	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	84462	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%


Target Compounds					Qvalue
13) Acetone	2.32	43	8045	3.339 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU021419\
Data File : VU029482.D
Acq On : 15 Feb 2019 01:51
Operator : JC/SP
Sample : K1438-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESXE3

Quant Time: Feb 15 04:09:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Feb 15 01:55:09 2019
Response via : Initial Calibration

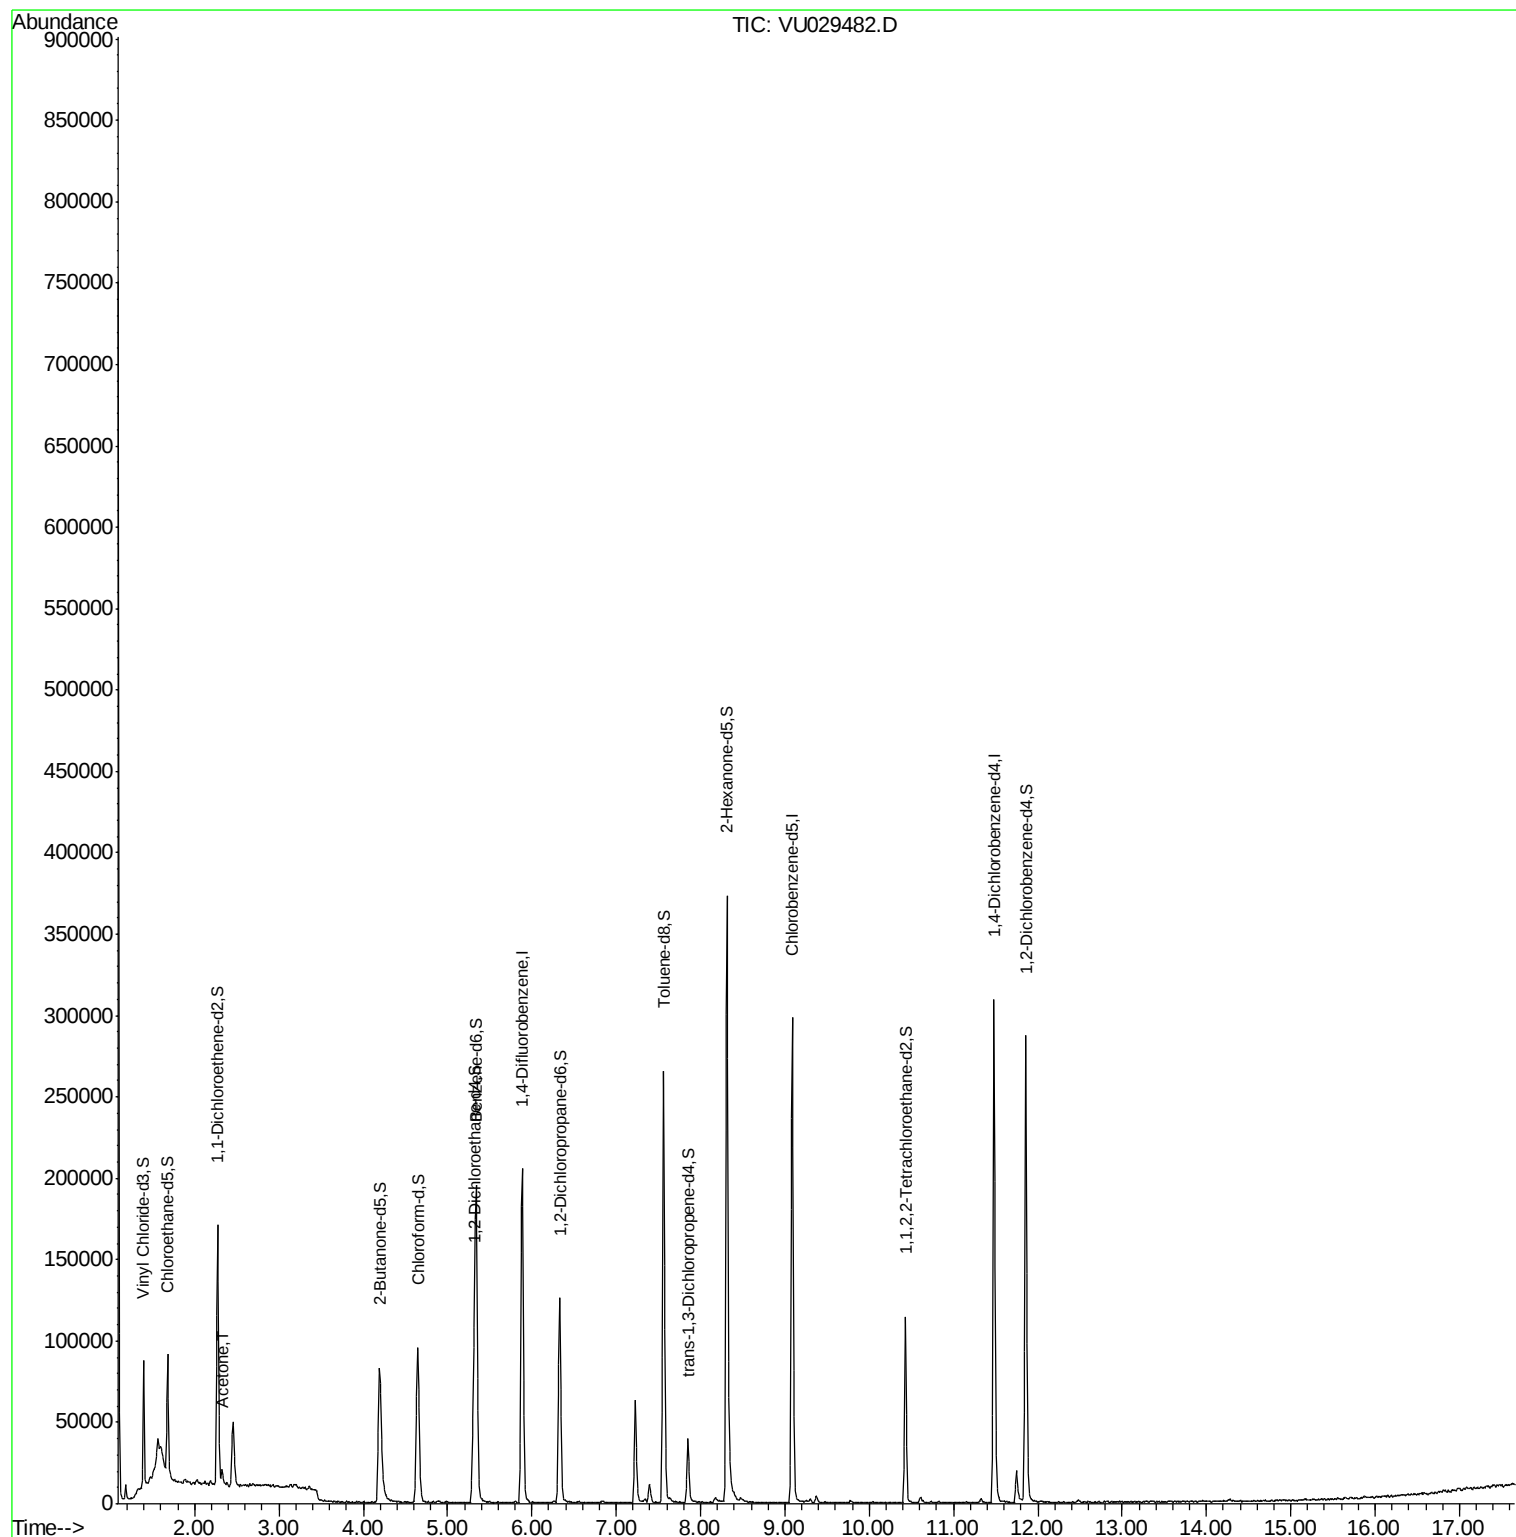

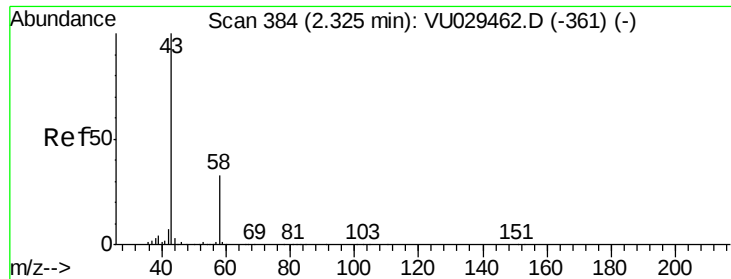

#13

Acetone

Concen: 3.339 ug/L

RT: 2.32 min Scan# 384

Delta R.T. -0.00 min

Lab File: VU029482.D

Acq: 15 Feb 2019 01:51

Instrument :

MSVOA_U

ClientSampleId :

ESXE3

Tgt Ion: 43 Resp: 8045

Ion Ratio Lower Upper

43 100

58 33.3 0.0 65.0

