

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021422\
 Data File : VU047135.D
 Acq On : 14 Feb 2022 16:28
 Operator : SY/MD
 Sample : N1205-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-EDBCP-WS

Quant Time: Feb 18 11:02:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 15 03:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.118	96	55004	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.635	95	20588	0.966	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	20794	0.937	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.000%	
Target Compounds						
						Qvalue
56) 1,2-Dibromoethane	8.928	107	22263	1.910	ug/l	97
71) 1,2,3-Trichloropropane	10.825	75	16645	1.265	ug/l	86
86) 1,2-Dibromo-3-Chloropr...	12.999	75	1504	0.526	ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021422\
Data File : VU047135.D
Acq On : 14 Feb 2022 16:28
Operator : SY/MD
Sample : N1205-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Time: Feb 18 11:02:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 15 03:17:28 2022
Response via : Initial Calibration




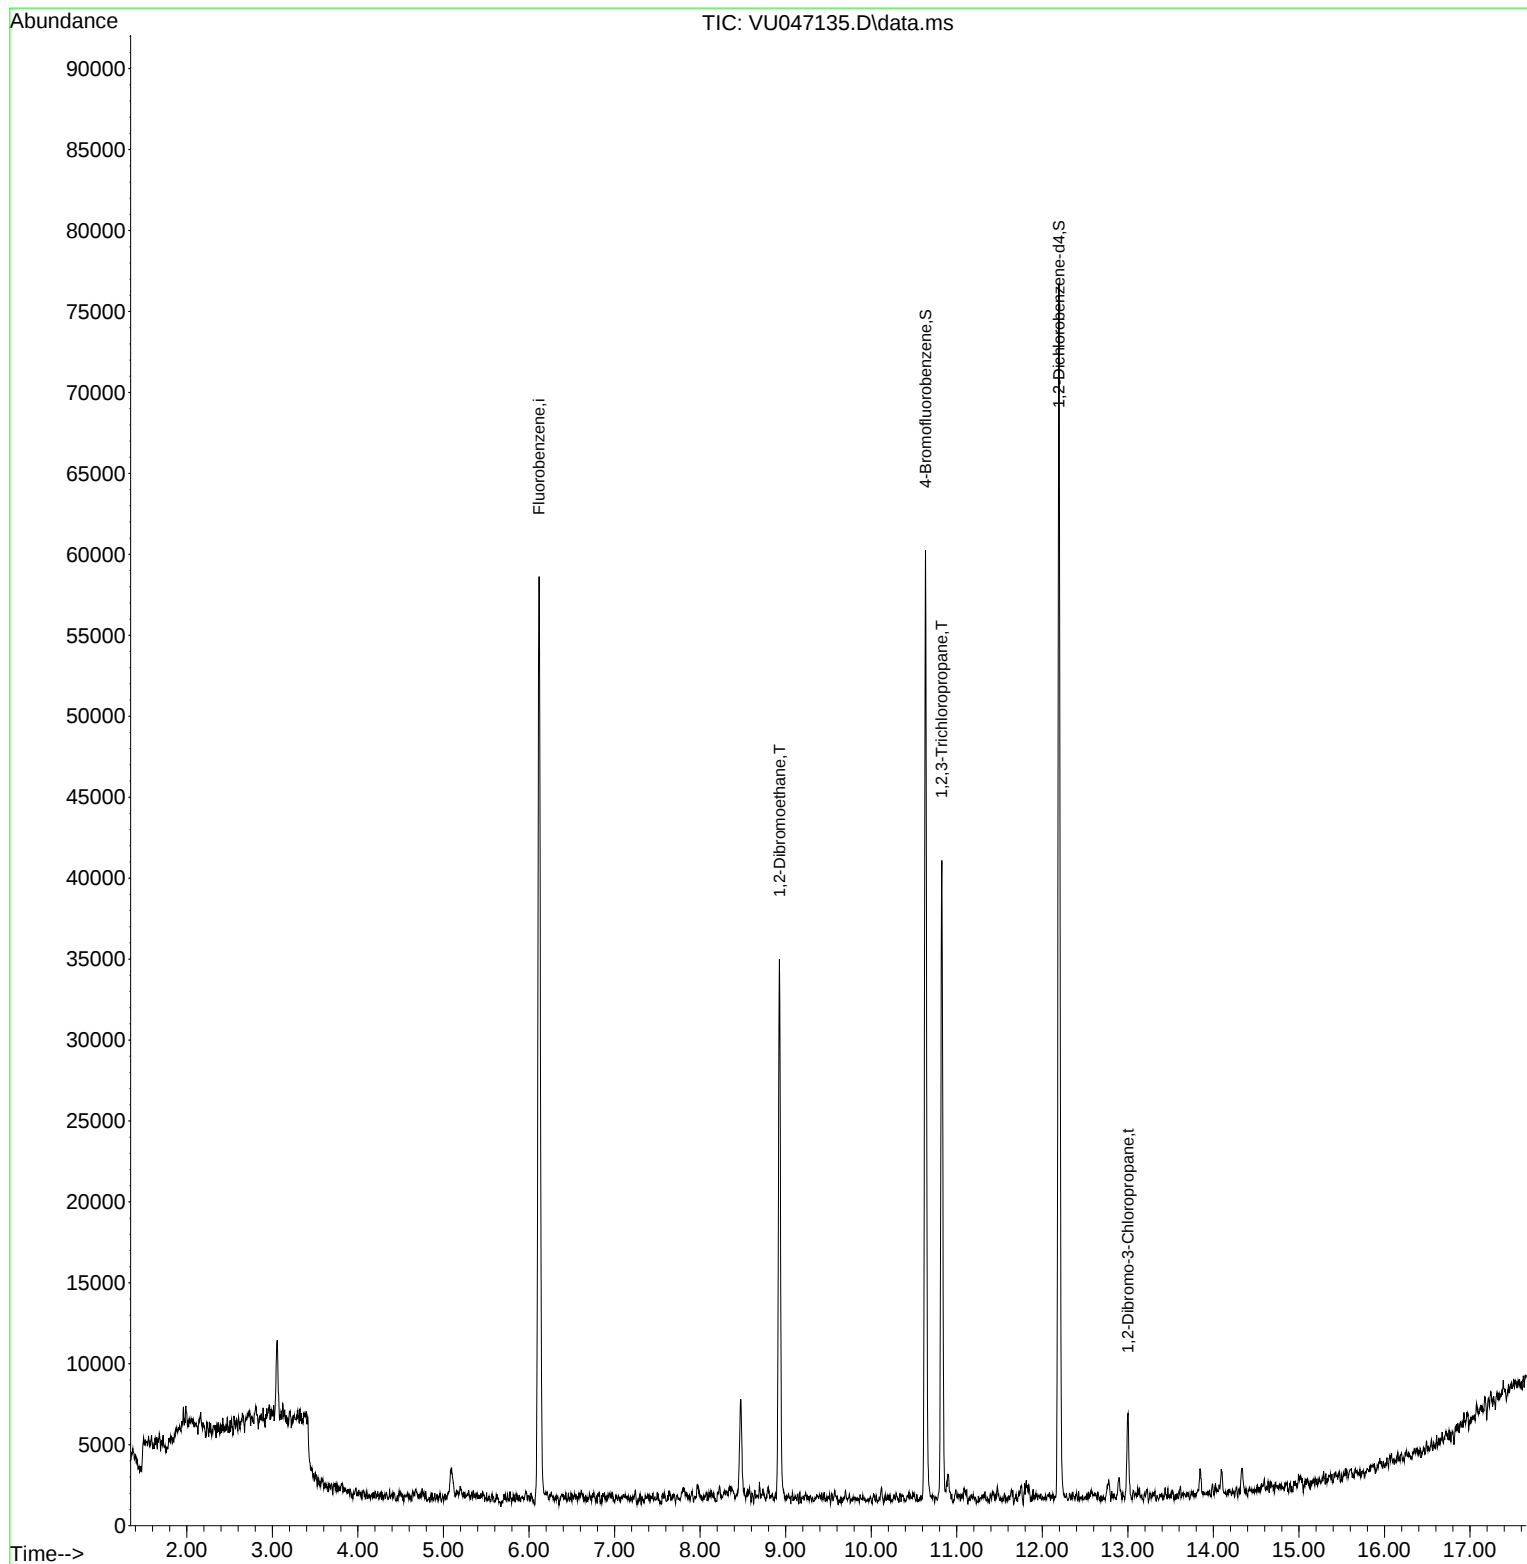


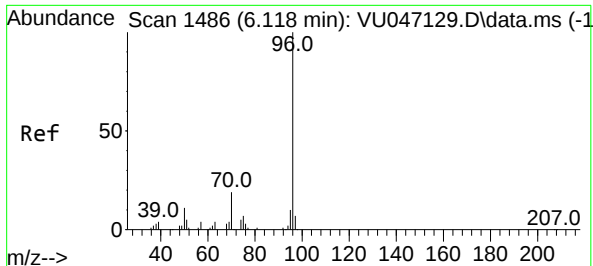

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 14
Delta R.T. -0.000 min
Lab File: VU047135.D
Acq: 14 Feb 2022 16:28




Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS


Tgt Ion: 96 Resp: 55004
Ion Ratio Lower Upper
96 100
70 20.5 16.8 25.2
95 8.9 7.3 10.9
97 6.4 0.0 0.0#

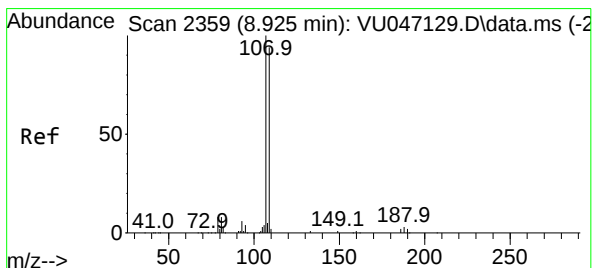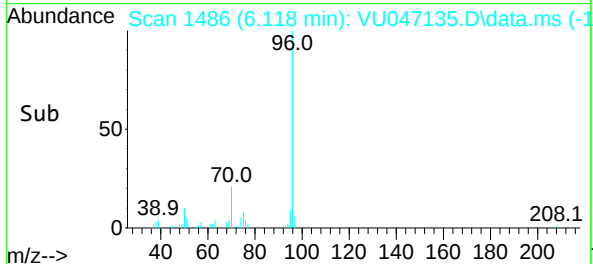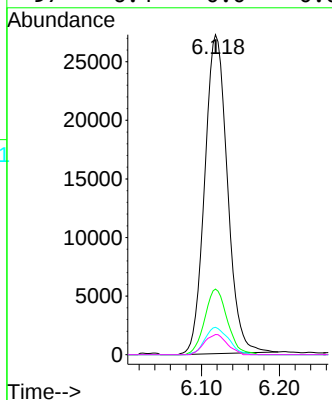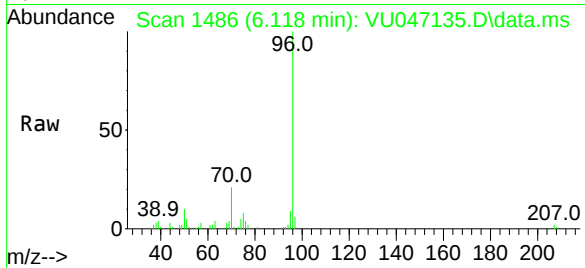

#56
1,2-Dibromoethane
Concen: 1.910 ug/l
RT: 8.928 min Scan# 2360
Delta R.T. 0.003 min
Lab File: VU047135.D
Acq: 14 Feb 2022 16:28

Tgt Ion: 107 Resp: 22263
Ion Ratio Lower Upper
107 100
109 95.1 0.0 185.0


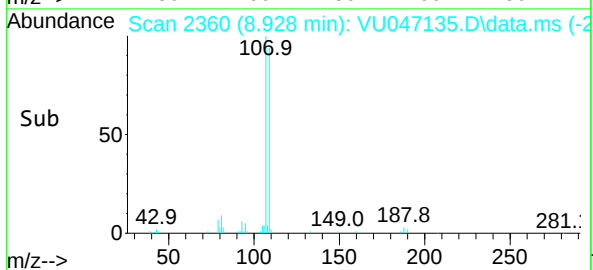
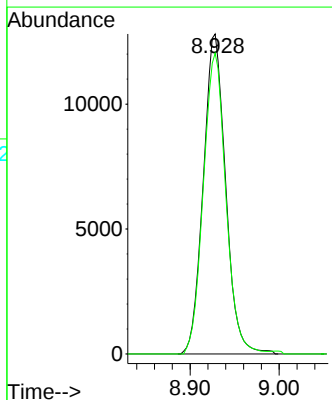
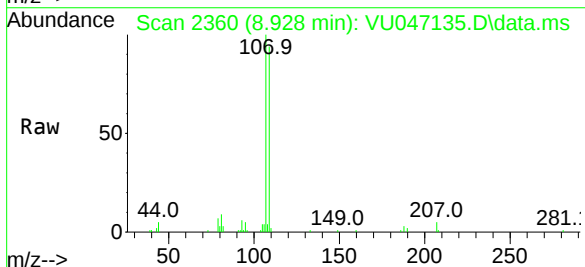


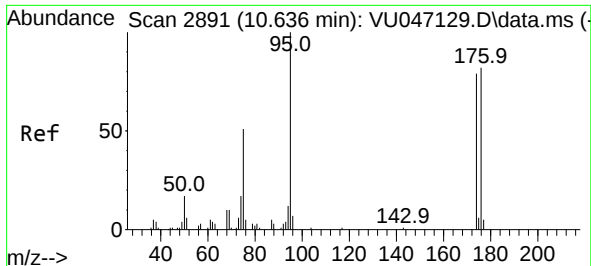

#57
4-Bromofluorobenzene
Concen: 0.966 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. -0.000 min
Lab File: VU047135.D
Acq: 14 Feb 2022 16:28




Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS


Tgt Ion: 95 Resp: 20588
Ion Ratio Lower Upper
95 100
174 78.9 56.6 84.8
176 78.0 54.3 81.5

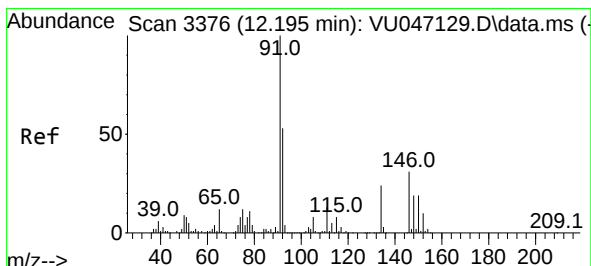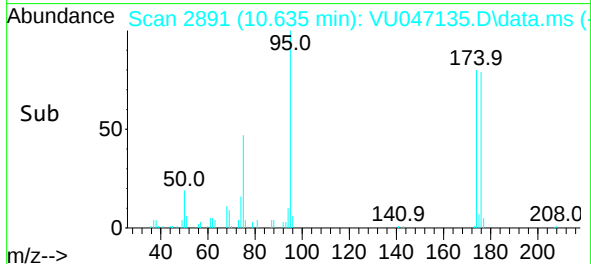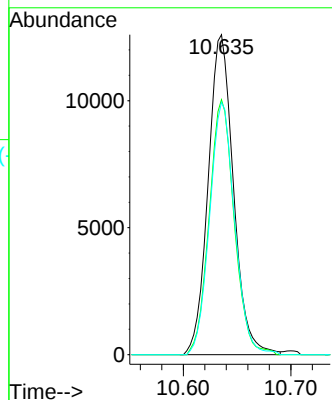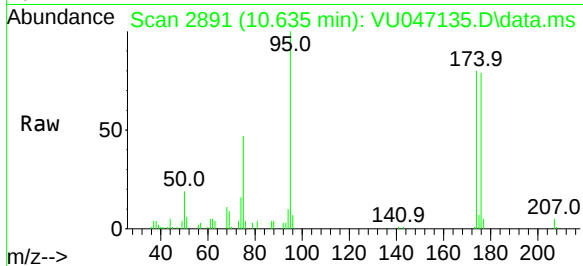

#68
1,2-Dichlorobenzene-d4
Concen: 0.937 ug/l
RT: 12.195 min Scan# 3376
Delta R.T. -0.000 min
Lab File: VU047135.D
Acq: 14 Feb 2022 16:28

Tgt Ion: 152 Resp: 20794
Ion Ratio Lower Upper
152 100
115 62.1 0.0 251.0
150 156.6 0.0 613.8


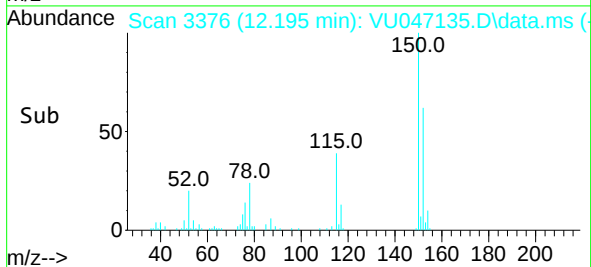
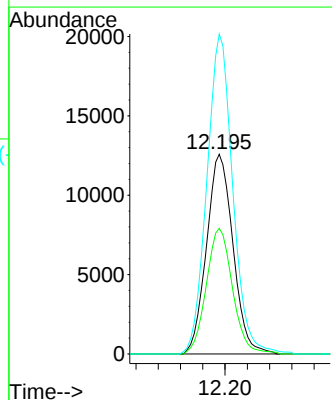
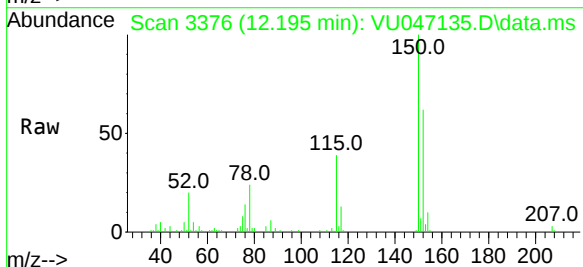


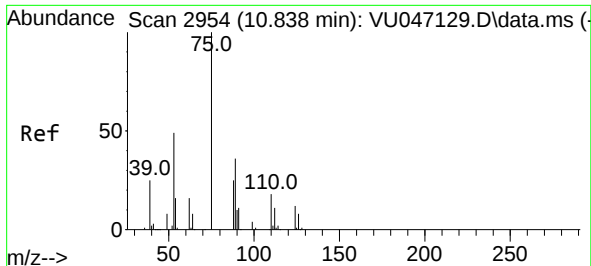

#71
1,2,3-Trichloropropane
Concen: 1.265 ug/l
RT: 10.825 min Scan# 2950
Delta R.T. -0.013 min
Lab File: VU047135.D
Acq: 14 Feb 2022 16:28

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Tgt Ion: 75	Resp: 16645
Ion Ratio	Lower Upper
75 100	
77 33.6	0.0 105.6
110 35.4	0.0 71.2
97 20.5	0.0 36.8

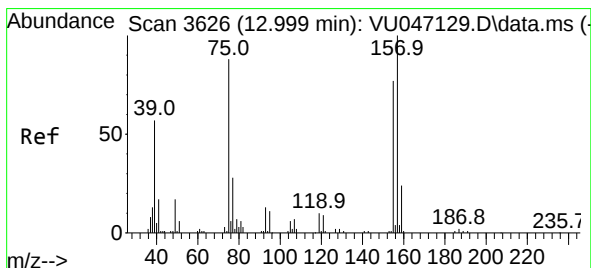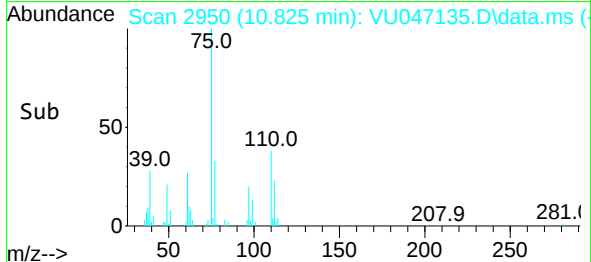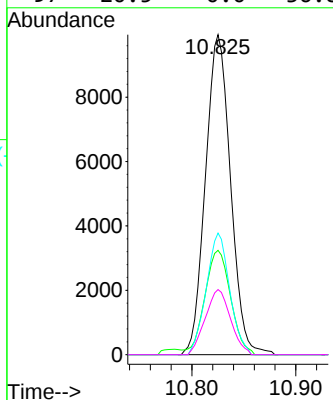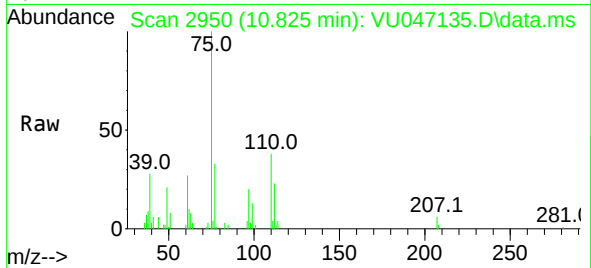

#86
1,2-Dibromo-3-Chloropropane
Concen: 0.526 ug/l
RT: 12.999 min Scan# 3626
Delta R.T. -0.000 min
Lab File: VU047135.D
Acq: 14 Feb 2022 16:28

Tgt Ion: 75	Resp: 1504
Ion Ratio	Lower Upper
75 100	
155 84.4	57.8 86.8
157 102.2	75.1 112.7

