

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021422\
 Data File : VU047139.D
 Acq On : 14 Feb 2022 18:26
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Feb 15 03:52:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 15 03:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	54217	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.635	95	19944	0.950	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	20416	0.933	ug/l	0.00
Spiked Amount 1.000			Recovery	=	93.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021422\
Data File : VU047139.D
Acq On : 14 Feb 2022 18:26
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Feb 15 03:52:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 15 03:17:28 2022
Response via : Initial Calibration




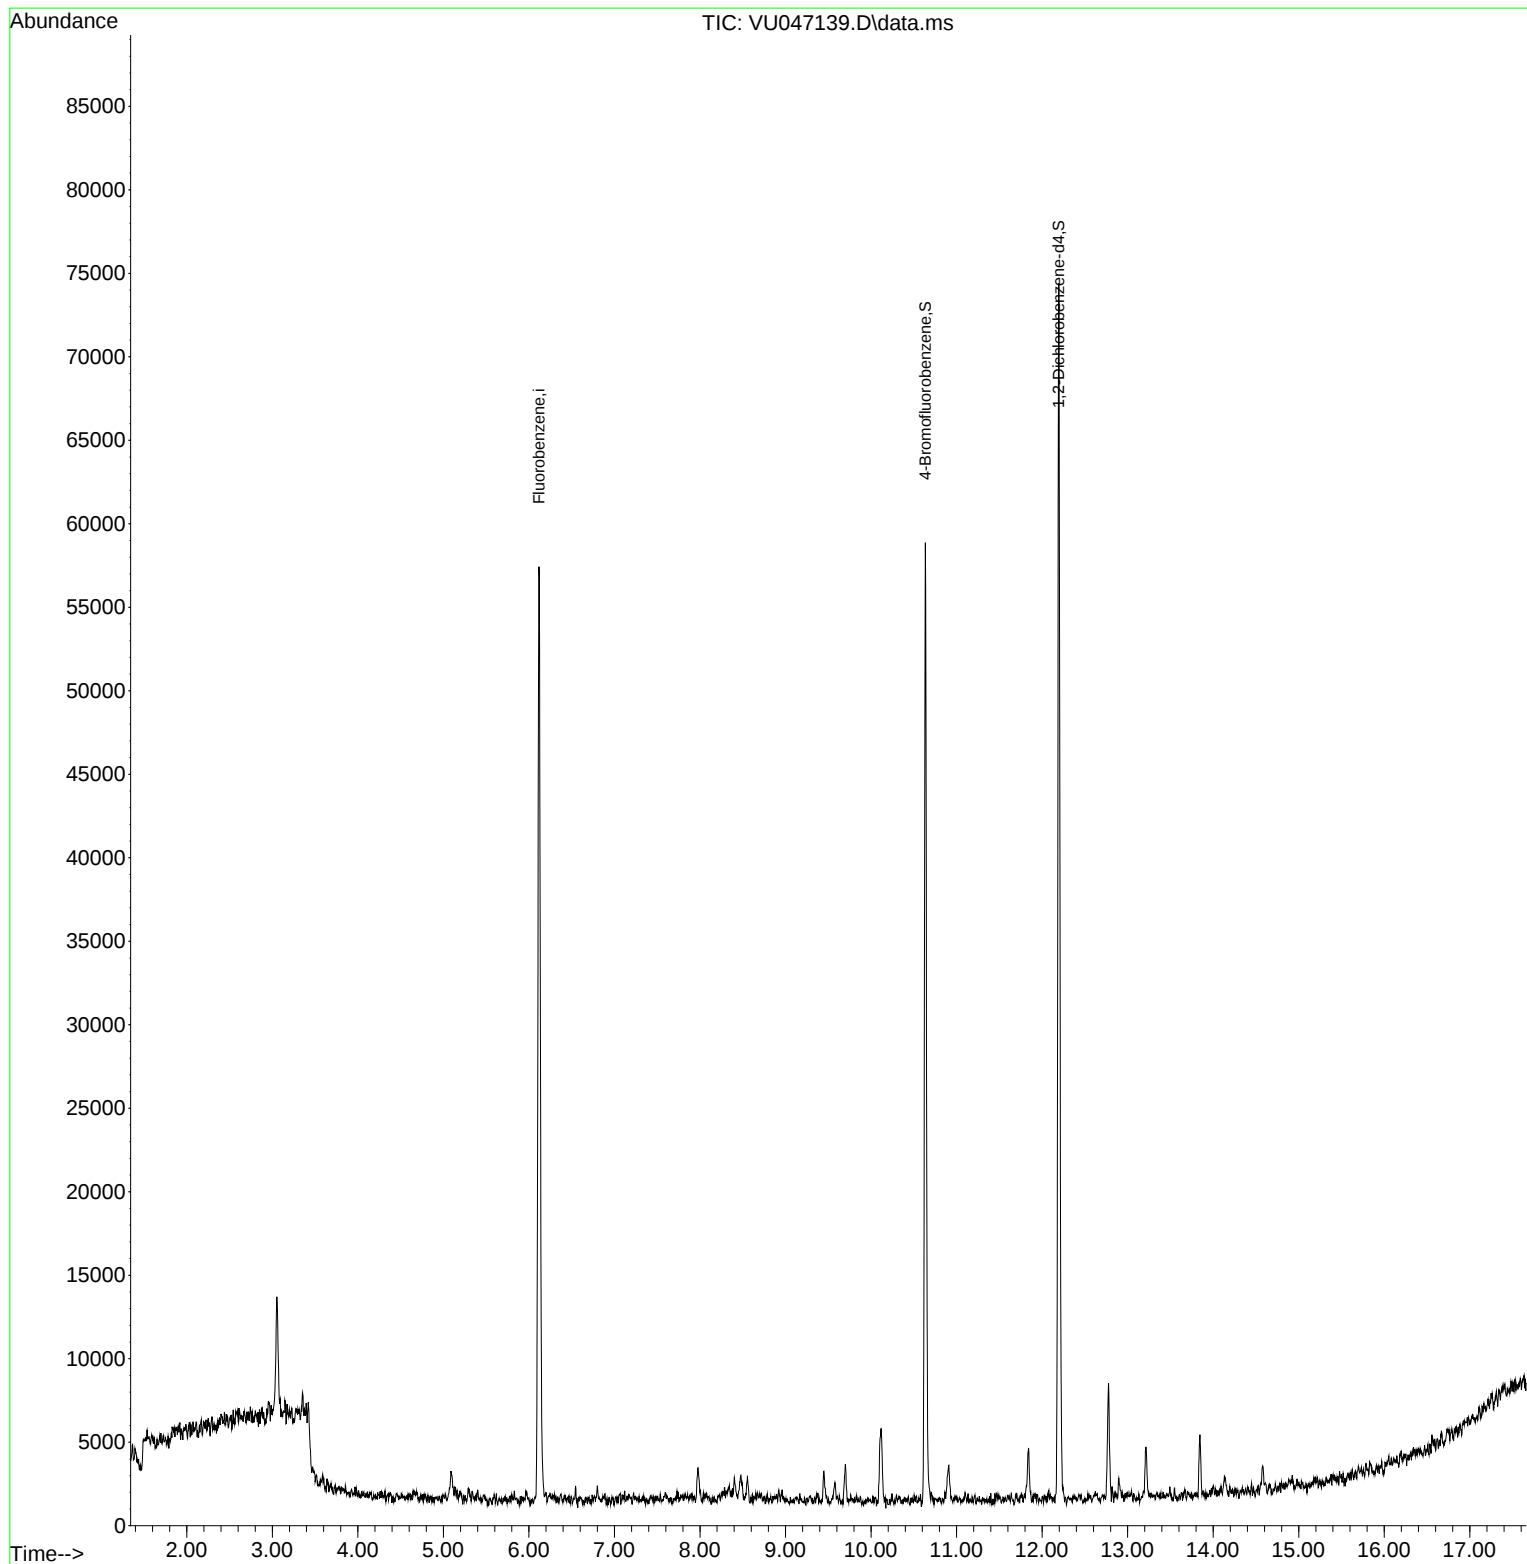


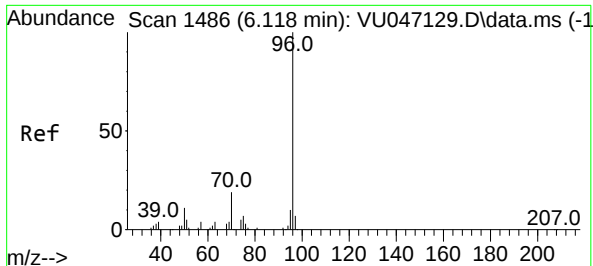

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. -0.000 min
Lab File: VU047139.D
Acq: 14 Feb 2022 18:26




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion: 96	Resp: 54217
Ion Ratio	Lower Upper
96 100	
70 19.7	16.8 25.2
95 8.7	7.3 10.9
97 6.2	0.0 0.0#

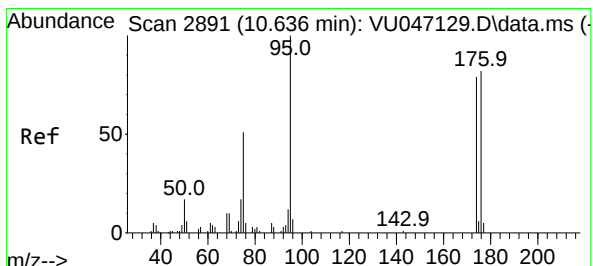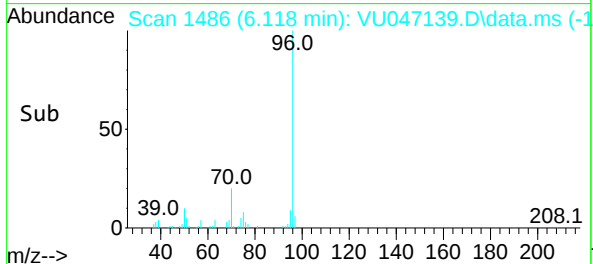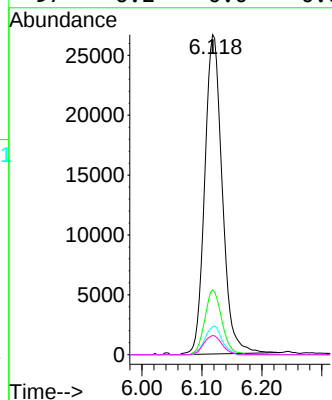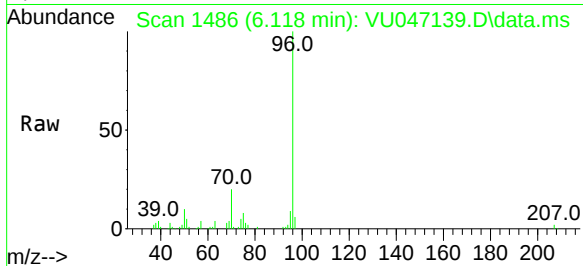

#57
4-Bromofluorobenzene
Concen: 0.950 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. -0.000 min
Lab File: VU047139.D
Acq: 14 Feb 2022 18:26

Tgt Ion: 95	Resp: 19944
Ion Ratio	Lower Upper
95 100	
174 77.7	56.6 84.8
176 78.4	54.3 81.5

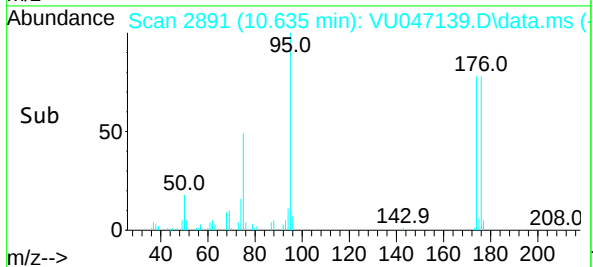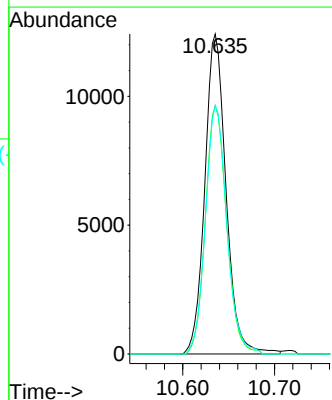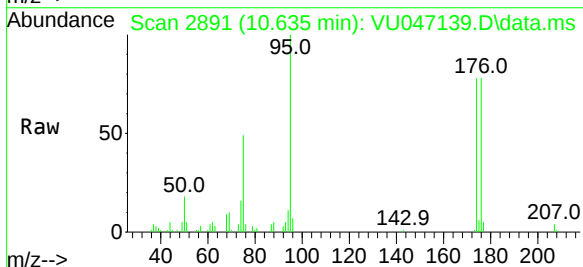

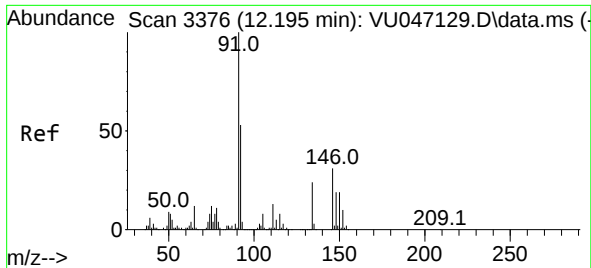

#68

1,2-Dichlorobenzene-d4

Concen: 0.933 ug/l

RT: 12.195 min Scan# 31

Delta R.T. -0.000 min

Lab File: VU047139.D


Acq: 14 Feb 2022 18:26

Instrument :

MSVOA_U

ClientSampleId :

VIBLK

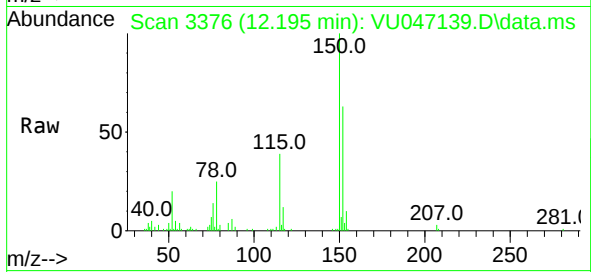

Tgt Ion:152 Resp: 20416

Ion Ratio Lower Upper

152 100

115 61.6 0.0 251.0

150 153.9 0.0 613.8

