


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021422\
Data File : VU047124.D
Acq On : 14 Feb 2022 09:02
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Feb 15 03:17:28 2022

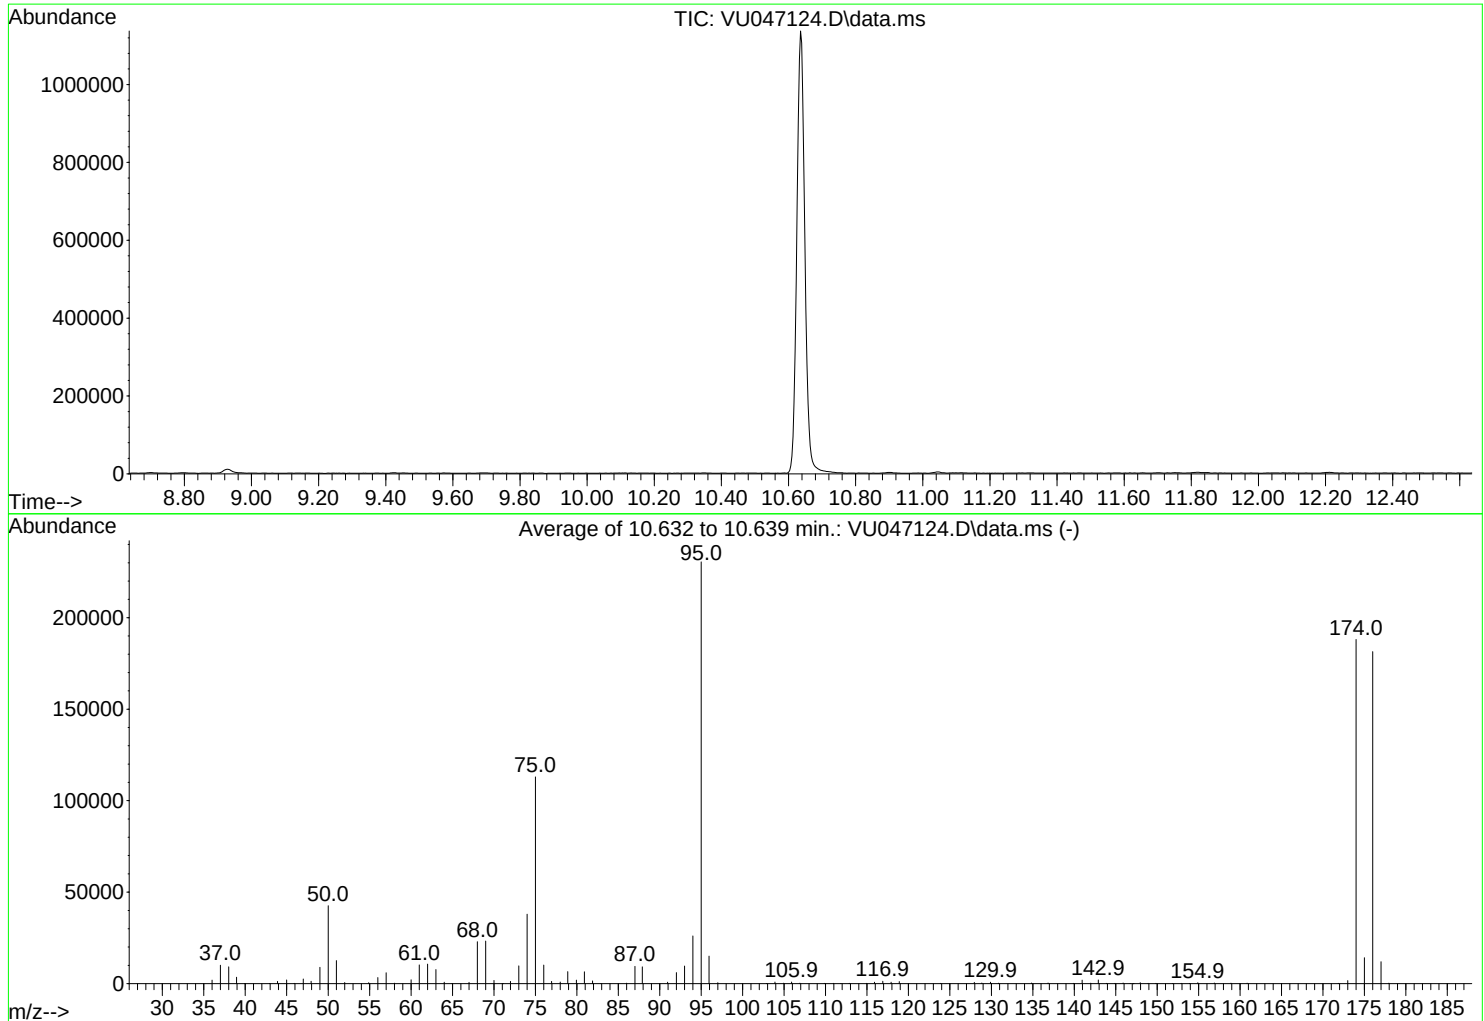

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	42619	PASS
75	95	30	60	49.0	112981	PASS
95	95	100	100	100.0	230507	PASS
96	95	5	9	6.5	15037	PASS
173	174	0.00	2	0.9	1635	PASS
174	95	50	100	81.6	188053	PASS
175	174	5	9	7.5	14181	PASS
176	174	95	101	96.5	181461	PASS
177	176	5	9	6.6	11977	PASS