

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
 Data File : VU053098.D
 Acq On : 14 Feb 2023 15:34
 Operator : JC/MD
 Sample : VU0214WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK046

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

Signal : TIC: VU053098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	43	52	71	rBV	225060	304034	25.27%	3.382%
2	1.598	151	158	173	rVB	161810	190099	15.80%	2.114%
3	1.913	249	256	273	rBV	132696	176050	14.63%	1.958%
4	2.563	447	458	476	rVB	258911	423844	35.23%	4.714%
5	3.039	599	606	618	rVB6	3155	6054	0.50%	0.067%
6	3.347	697	702	705	rBV2	1032	898	0.07%	0.010%
7	3.556	762	767	770	rBV	699	585	0.05%	0.007%
8	3.576	770	773	775	rBV3	362	256	0.02%	0.003%
9	3.756	825	829	830	rBV2	444	309	0.03%	0.003%
10	3.955	889	891	896	rBV2	342	277	0.02%	0.003%
11	4.016	907	910	912	rBV2	402	272	0.02%	0.003%
12	4.077	927	929	933	rVB	409	250	0.02%	0.003%
13	4.148	946	951	952	rBV2	476	404	0.03%	0.004%
14	4.254	981	984	987	rBV3	384	313	0.03%	0.003%
15	4.424	1034	1037	1040	rBV2	613	480	0.04%	0.005%
16	4.624	1083	1099	1127	rBV	75082	205331	17.07%	2.284%
17	4.907	1181	1187	1190	rBV3	675	723	0.06%	0.008%
18	5.058	1218	1234	1254	rBV	223380	492347	40.92%	5.476%
19	5.193	1271	1276	1279	rBV5	534	461	0.04%	0.005%
20	5.264	1291	1298	1302	rBV5	773	999	0.08%	0.011%
21	5.283	1302	1304	1307	rVB3	534	320	0.03%	0.004%
22	5.331	1316	1319	1322	rBV3	351	287	0.02%	0.003%
23	5.373	1325	1332	1335	rBV4	1241	1283	0.11%	0.014%
24	5.489	1367	1368	1371	rVV2	389	242	0.02%	0.003%
25	5.543	1381	1385	1387	rBV2	413	256	0.02%	0.003%
26	5.559	1388	1390	1394	rVB3	480	279	0.02%	0.003%
27	5.720	1417	1440	1464	rBV2	444242	1203137	100.00%	13.382%
28	5.987	1520	1523	1528	rBV3	517	379	0.03%	0.004%
29	6.042	1537	1540	1544	rVV3	461	385	0.03%	0.004%
30	6.064	1544	1547	1551	rVB2	408	254	0.02%	0.003%
31	6.100	1557	1558	1563	rVB	490	315	0.03%	0.004%
32	6.138	1568	1570	1574	rVB2	617	253	0.02%	0.003%
33	6.244	1586	1603	1625	rBV	323186	609930	50.69%	6.784%
34	6.402	1648	1652	1656	rVB4	728	719	0.06%	0.008%
35	6.424	1656	1659	1661	rBV2	599	468	0.04%	0.005%
36	6.521	1685	1689	1690	rBV4	1078	842	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
 Data File : VU053098.D
 Acq On : 14 Feb 2023 15:34
 Operator : JC/MD
 Sample : VU0214WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK046

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	6.685	1726	1740	1760	rBV	285378	549554	45.68%	6.112%
38	6.894	1801	1805	1810	rBV3	630	583	0.05%	0.006%
39	6.939	1817	1819	1824	rVB2	569	345	0.03%	0.004%
40	6.968	1826	1828	1831	rBV	503	289	0.02%	0.003%
41	7.077	1858	1862	1866	rBV2	557	471	0.04%	0.005%
42	7.180	1886	1894	1900	rBV5	1479	2397	0.20%	0.027%
43	7.479	1985	1987	1991	rVB2	464	272	0.02%	0.003%
44	7.559	1999	2012	2030	rBV	176788	307509	25.56%	3.420%
45	7.691	2046	2053	2058	rBV7	779	1159	0.10%	0.013%
46	7.791	2075	2084	2088	rBV7	1209	1880	0.16%	0.021%
47	7.894	2101	2116	2139	rBV	568589	975014	81.04%	10.845%
48	8.067	2168	2170	2174	rBV3	457	316	0.03%	0.004%
49	8.116	2182	2185	2190	rBV2	518	419	0.03%	0.005%
50	8.174	2190	2203	2222	rBV	118926	202370	16.82%	2.251%
51	8.325	2245	2250	2255	rBV4	523	590	0.05%	0.007%
52	8.357	2256	2260	2263	rBV3	306	262	0.02%	0.003%
53	8.392	2269	2271	2275	rBV2	455	346	0.03%	0.004%
54	8.431	2279	2283	2288	rVB3	275	267	0.02%	0.003%
55	8.521	2306	2311	2315	rBV4	525	546	0.05%	0.006%
56	8.553	2315	2321	2325	rBV4	823	1083	0.09%	0.012%
57	8.630	2333	2345	2374	rBV2	258631	479498	39.85%	5.333%
58	8.952	2442	2445	2448	rVB2	587	337	0.03%	0.004%
59	9.029	2466	2469	2471	rBV2	462	299	0.02%	0.003%
60	9.090	2485	2488	2492	rBV3	390	393	0.03%	0.004%
61	9.325	2559	2561	2564	rBV	368	267	0.02%	0.003%
62	9.411	2576	2588	2611	rBV	435102	719853	59.83%	8.007%
63	9.553	2629	2632	2633	rBV2	505	240	0.02%	0.003%
64	9.630	2650	2656	2660	rBV2	531	572	0.05%	0.006%
65	9.653	2660	2663	2666	rVB2	408	246	0.02%	0.003%
66	9.678	2667	2671	2672	rBV2	401	262	0.02%	0.003%
67	9.698	2672	2677	2682	rVV4	1374	1488	0.12%	0.017%
68	9.820	2713	2715	2720	rVB2	494	369	0.03%	0.004%
69	9.948	2752	2755	2758	rBV2	326	305	0.03%	0.003%
70	9.984	2763	2766	2769	rBV2	459	361	0.03%	0.004%
71	10.106	2796	2804	2813	rBV6	1727	2919	0.24%	0.032%
72	10.173	2822	2825	2829	rVB2	436	357	0.03%	0.004%
73	10.199	2829	2833	2837	rBV2	390	359	0.03%	0.004%
74	10.257	2848	2851	2856	rVB4	493	419	0.03%	0.005%
75	10.341	2874	2877	2880	rBV3	466	290	0.02%	0.003%
76	10.424	2900	2903	2908	rVB3	439	312	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
 Data File : VU053098.D
 Acq On : 14 Feb 2023 15:34
 Operator : JC/MD
 Sample : VU0214WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK046

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

77	10.479	2914	2920	2926	rBV4	1158	1727	0.14%	0.019%
78	10.524	2932	2934	2937	rBV2	383	267	0.02%	0.003%
79	10.575	2945	2950	2956	rVB3	718	812	0.07%	0.009%
80	10.752	2990	3005	3021	rBV	341029	557456	46.33%	6.200%
81	10.849	3033	3035	3041	rVB2	516	426	0.04%	0.005%
82	10.939	3056	3063	3066	rBV2	331	477	0.04%	0.005%
83	11.087	3104	3109	3117	rVV3	1511	2019	0.17%	0.022%
84	11.305	3173	3177	3178	rBV	504	360	0.03%	0.004%
85	11.469	3219	3228	3232	rBV5	2001	2782	0.23%	0.031%
86	11.746	3306	3314	3320	rBV5	2374	3442	0.29%	0.038%
87	11.807	3320	3333	3354	rBV	439361	703682	58.49%	7.827%
88	12.048	3405	3408	3413	rVB2	493	313	0.03%	0.003%
89	12.186	3439	3451	3476	rBV	487176	795399	66.11%	8.847%
90	12.566	3566	3569	3578	rVB4	432	517	0.04%	0.006%
91	12.723	3615	3618	3622	rBV3	340	298	0.02%	0.003%
92	12.800	3638	3642	3646	rVB4	548	435	0.04%	0.005%
93	13.196	3761	3765	3766	rBV2	336	247	0.02%	0.003%
94	13.222	3767	3773	3781	rVB7	2499	3828	0.32%	0.043%
95	13.389	3823	3825	3829	rBV	327	244	0.02%	0.003%
96	13.733	3928	3932	3935	rBV	356	306	0.03%	0.003%
97	13.839	3957	3965	3974	rBV4	5375	8260	0.69%	0.092%
98	13.939	3995	3996	4002	rVB4	411	269	0.02%	0.003%
99	14.090	4034	4043	4053	rVB2	12096	19337	1.61%	0.215%
100	14.324	4109	4116	4126	rVB4	6079	9667	0.80%	0.108%




Sum of corrected areas: 8990723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
Data File : VU053098.D
Acq On : 14 Feb 2023 15:34
Operator : JC/MD
Sample : VU0214WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK046

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

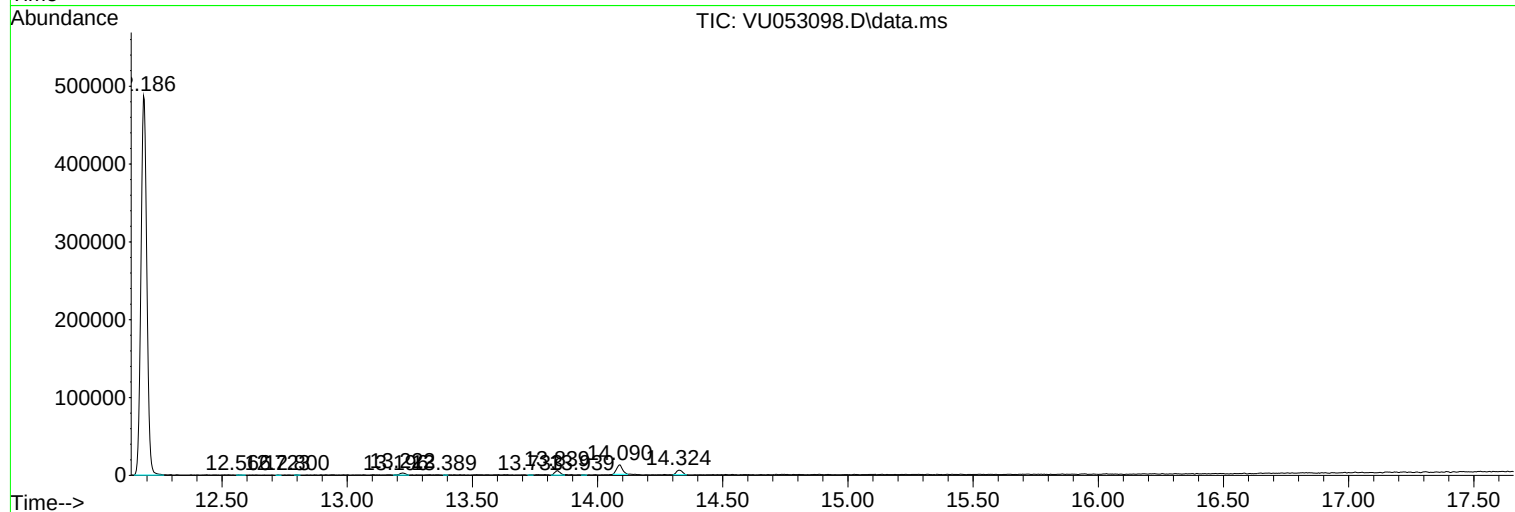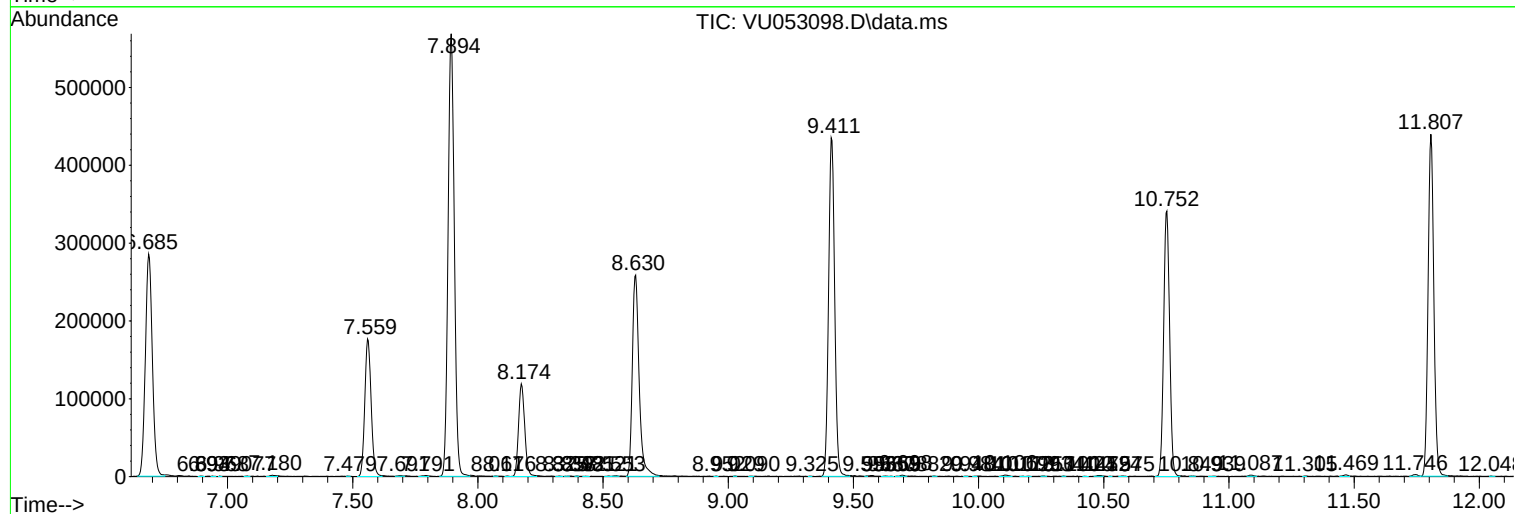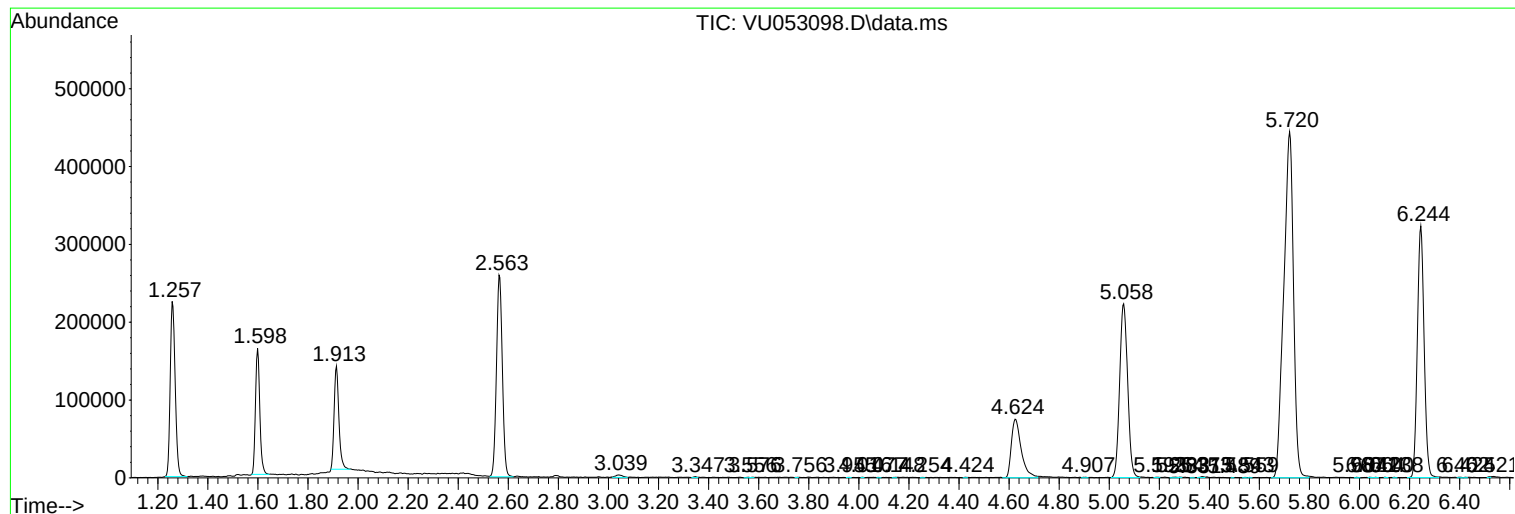

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
Data File : VU053098.D
Acq On : 14 Feb 2023 15:34
Operator : JC/MD
Sample : VU0214WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK046

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
Data File : VU053098.D
Acq On : 14 Feb 2023 15:34
Operator : JC/MD
Sample : VU0214WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK046

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------