

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
 Data File : VU053100.D
 Acq On : 14 Feb 2023 17:38
 Operator : JC/MD
 Sample : 01488-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M

Title : VOC Analysis

Signal : TIC: VU053100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	44	52	66	rVB	92976	117756	10.13%	1.394%
2	1.598	151	158	173	rVB	147369	170910	14.70%	2.024%
3	1.913	249	256	277	rVB	124894	170293	14.65%	2.017%
4	2.566	448	459	474	rVB	237946	390053	33.55%	4.619%
5	2.949	574	578	579	rBV3	547	373	0.03%	0.004%
6	3.077	616	618	622	rVB3	472	245	0.02%	0.003%
7	3.103	622	626	628	rBV	519	295	0.03%	0.003%
8	3.447	729	733	735	rBV	405	317	0.03%	0.004%
9	3.495	746	748	752	rBV2	331	277	0.02%	0.003%
10	3.627	787	789	792	rVB	489	275	0.02%	0.003%
11	3.666	795	801	807	rBV3	453	625	0.05%	0.007%
12	3.997	900	904	906	rBV3	447	367	0.03%	0.004%
13	4.077	925	929	932	rBV3	461	398	0.03%	0.005%
14	4.167	952	957	959	rVV2	450	351	0.03%	0.004%
15	4.206	966	969	971	rBV2	502	275	0.02%	0.003%
16	4.325	1003	1006	1008	rBV	265	210	0.02%	0.002%
17	4.396	1023	1028	1029	rBV2	574	479	0.04%	0.006%
18	4.547	1070	1075	1077	rBV3	363	240	0.02%	0.003%
19	4.624	1085	1099	1130	rBV	75803	207037	17.81%	2.452%
20	4.942	1195	1198	1200	rBV3	385	249	0.02%	0.003%
21	5.058	1217	1234	1258	rBV	217467	482015	41.46%	5.708%
22	5.170	1267	1269	1274	rVB	493	314	0.03%	0.004%
23	5.318	1313	1315	1319	rBV2	470	322	0.03%	0.004%
24	5.421	1344	1347	1351	rVB3	390	272	0.02%	0.003%
25	5.476	1358	1364	1369	rVB4	533	618	0.05%	0.007%
26	5.505	1369	1373	1374	rBV2	470	292	0.03%	0.003%
27	5.720	1419	1440	1461	rBV2	433180	1162539	100.00%	13.767%
28	5.910	1494	1499	1501	rBV5	452	388	0.03%	0.005%
29	6.199	1586	1589	1590	rBV	411	262	0.02%	0.003%
30	6.244	1590	1603	1626	rVV	307562	577152	49.65%	6.835%
31	6.453	1665	1668	1672	rBV3	331	271	0.02%	0.003%
32	6.524	1683	1690	1692	rBV5	1180	1072	0.09%	0.013%
33	6.585	1705	1709	1713	rBV4	272	298	0.03%	0.004%
34	6.608	1713	1716	1720	rVB2	347	264	0.02%	0.003%
35	6.685	1724	1740	1763	rBV	271197	530532	45.64%	6.282%
36	6.903	1806	1808	1811	rVV	458	276	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
 Data File : VU053100.D
 Acq On : 14 Feb 2023 17:38
 Operator : JC/MD
 Sample : 01488-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

37	6.981	1829	1832	1834	rVB3	480	242	0.02%	0.003%
38	6.997	1834	1837	1840	rBV3	371	292	0.03%	0.003%
39	7.103	1862	1870	1872	rBV3	507	628	0.05%	0.007%
40	7.241	1911	1913	1918	rVB3	390	308	0.03%	0.004%
41	7.350	1944	1947	1949	rBV	475	232	0.02%	0.003%
42	7.418	1965	1968	1970	rBV2	416	351	0.03%	0.004%
43	7.463	1979	1982	1987	rBV3	513	473	0.04%	0.006%
44	7.563	1999	2013	2031	rVV	167723	298286	25.66%	3.532%
45	7.688	2047	2052	2054	rBV3	1130	1094	0.09%	0.013%
46	7.772	2074	2078	2079	rBV	471	306	0.03%	0.004%
47	7.794	2080	2085	2086	rBV3	809	674	0.06%	0.008%
48	7.894	2102	2116	2136	rBV	550157	940012	80.86%	11.132%
49	8.051	2161	2165	2171	rVB3	533	587	0.05%	0.007%
50	8.122	2185	2187	2190	rVB2	645	220	0.02%	0.003%
51	8.173	2190	2203	2223	rBV	115709	196967	16.94%	2.332%
52	8.546	2316	2319	2322	rBV3	846	501	0.04%	0.006%
53	8.630	2333	2345	2381	rBV2	253033	478640	41.17%	5.668%
54	8.845	2407	2412	2420	rBV2	419	597	0.05%	0.007%
55	8.881	2420	2423	2427	rVV3	394	252	0.02%	0.003%
56	9.138	2500	2503	2506	rVB3	508	285	0.02%	0.003%
57	9.212	2524	2526	2530	rBV2	322	280	0.02%	0.003%
58	9.283	2542	2548	2550	rBV4	613	518	0.04%	0.006%
59	9.415	2575	2589	2610	rBV	405412	680955	58.57%	8.064%
60	9.810	2710	2712	2717	rBV2	311	243	0.02%	0.003%
61	9.871	2726	2731	2732	rBV	299	261	0.02%	0.003%
62	9.910	2739	2743	2750	rBV4	497	536	0.05%	0.006%
63	10.074	2790	2794	2795	rBV	296	218	0.02%	0.003%
64	10.090	2797	2799	2802	rBV2	399	306	0.03%	0.004%
65	10.109	2802	2805	2807	rBV3	593	343	0.03%	0.004%
66	10.161	2817	2821	2825	rBV2	605	653	0.06%	0.008%
67	10.209	2830	2836	2838	rBV	313	306	0.03%	0.004%
68	10.238	2842	2845	2848	rBV2	372	273	0.02%	0.003%
69	10.325	2864	2872	2873	rBV2	286	261	0.02%	0.003%
70	10.514	2927	2931	2932	rBV	377	271	0.02%	0.003%
71	10.566	2943	2947	2948	rBV	357	254	0.02%	0.003%
72	10.640	2966	2970	2971	rBV2	310	232	0.02%	0.003%
73	10.752	2991	3005	3026	rBV	343517	547866	47.13%	6.488%
74	10.855	3034	3037	3041	rBV3	442	420	0.04%	0.005%
75	11.083	3102	3108	3115	rVB4	863	1345	0.12%	0.016%
76	11.119	3115	3119	3123	rVB3	413	348	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
 Data File : VU053100.D
 Acq On : 14 Feb 2023 17:38
 Operator : JC/MD
 Sample : 01488-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
 Title : VOC Analysis

77	11.231	3150	3154	3156	rBV	466	371	0.03%	0.004%
78	11.324	3180	3183	3185	rBV2	488	223	0.02%	0.003%
79	11.405	3205	3208	3210	rBV2	549	372	0.03%	0.004%
80	11.443	3217	3220	3221	rBV2	362	220	0.02%	0.003%
81	11.466	3221	3227	3234	rVV6	1697	2634	0.23%	0.031%
82	11.681	3288	3294	3296	rBV3	769	764	0.07%	0.009%
83	11.807	3321	3333	3352	rBV	418746	669561	57.59%	7.929%
84	11.958	3377	3380	3383	rVB2	466	298	0.03%	0.004%
85	12.013	3392	3397	3400	rBV3	451	474	0.04%	0.006%
86	12.189	3440	3452	3473	rVB	478323	773837	66.56%	9.164%
87	12.759	3626	3629	3632	rBV3	629	525	0.05%	0.006%
88	12.810	3643	3645	3648	rBV2	354	225	0.02%	0.003%
89	13.083	3726	3730	3731	rVB2	455	286	0.02%	0.003%
90	13.099	3731	3735	3742	rBV3	829	1044	0.09%	0.012%
91	13.215	3765	3771	3779	rBV6	2147	2777	0.24%	0.033%
92	13.276	3786	3790	3793	rBV4	495	340	0.03%	0.004%
93	13.418	3832	3834	3840	rVV4	444	379	0.03%	0.004%
94	13.524	3865	3867	3869	rBV2	482	216	0.02%	0.003%
95	13.800	3950	3953	3956	rBV2	389	302	0.03%	0.004%
96	14.090	4036	4043	4053	rBV3	5037	7308	0.63%	0.087%
97	14.260	4093	4096	4099	rBV2	594	489	0.04%	0.006%
98	14.331	4111	4118	4126	rVB7	3926	6191	0.53%	0.073%
99	14.723	4238	4240	4243	rBV2	530	368	0.03%	0.004%
100	14.987	4319	4322	4326	rBV3	732	651	0.06%	0.008%




Sum of corrected areas: 8444603

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
Data File : VU053100.D
Acq On : 14 Feb 2023 17:38
Operator : JC/MD
Sample : 01488-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

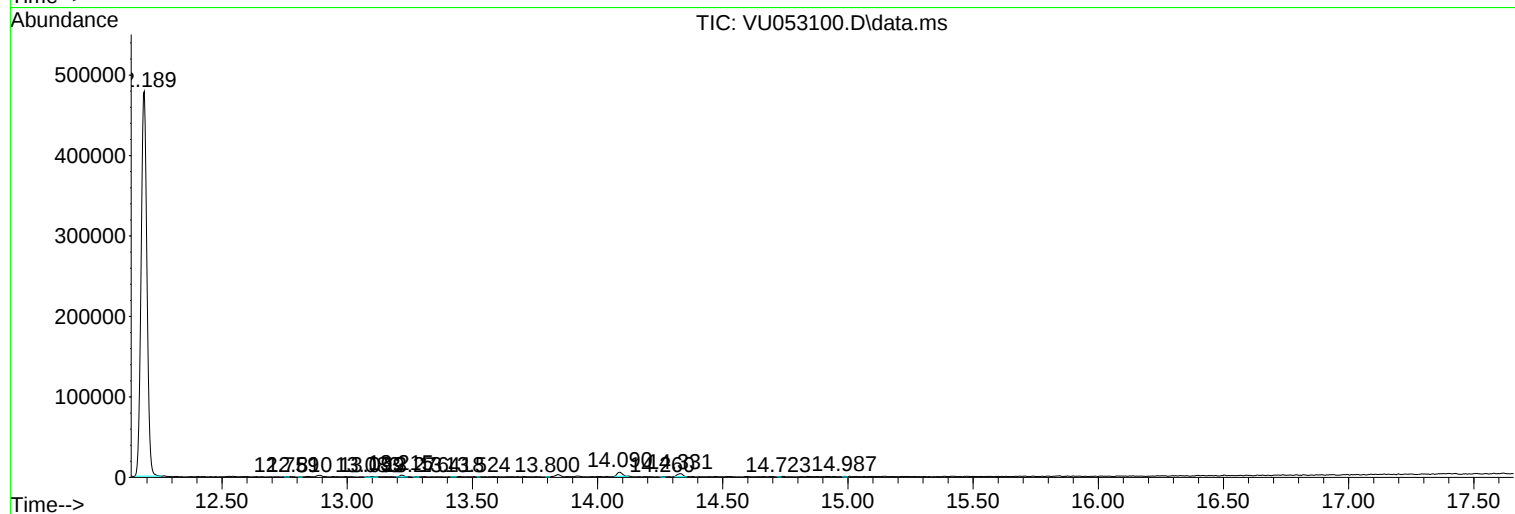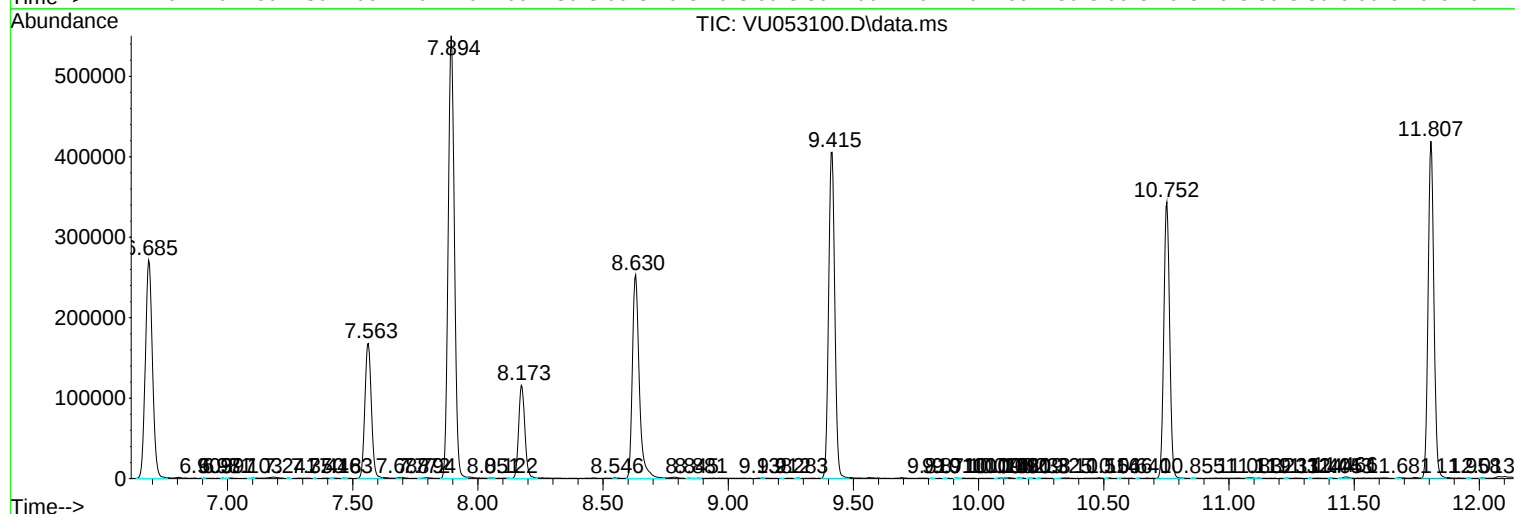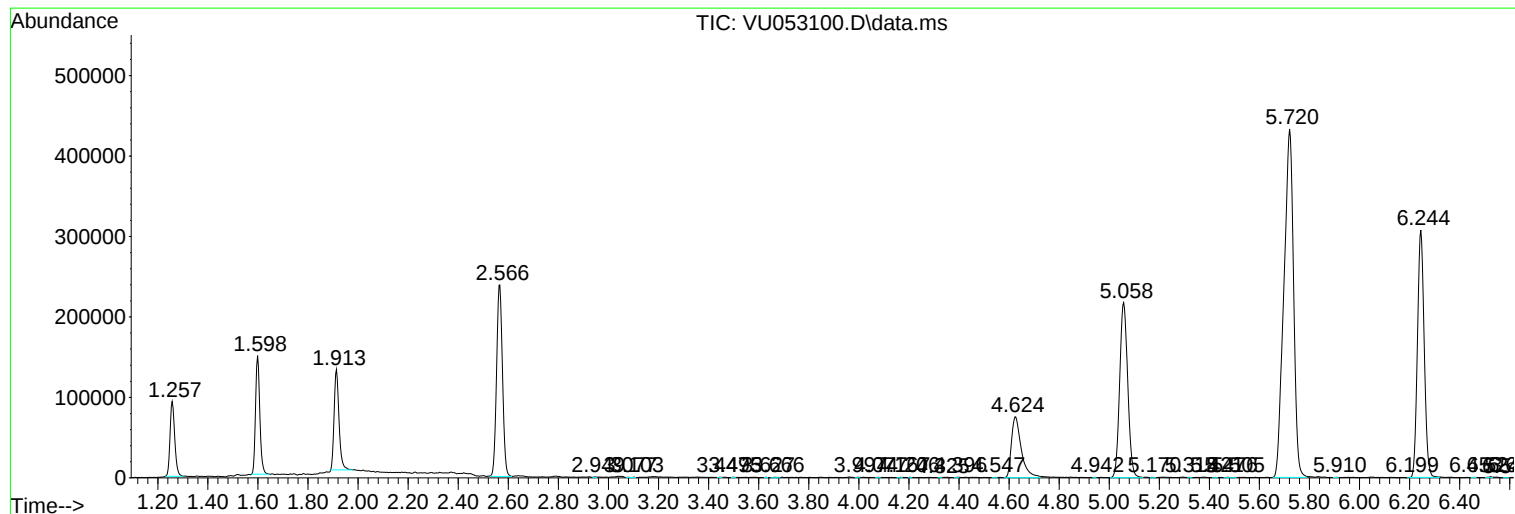

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
Data File : VU053100.D
Acq On : 14 Feb 2023 17:38
Operator : JC/MD
Sample : 01488-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
Data File : VU053100.D
Acq On : 14 Feb 2023 17:38
Operator : JC/MD
Sample : 01488-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------