
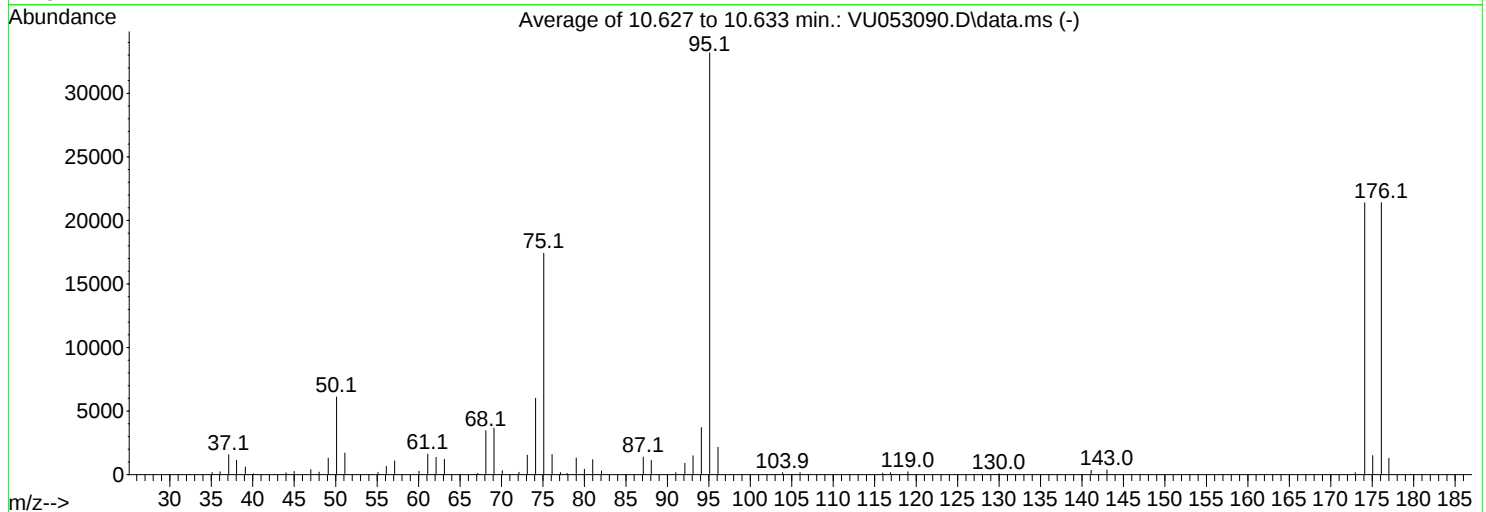


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021423\
Data File : VU053090.D
Acq On : 14 Feb 2023 09:52
Operator : JC/MD
Sample : BFB160
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB160

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis
Last Update : Wed Feb 15 00:41:46 2023

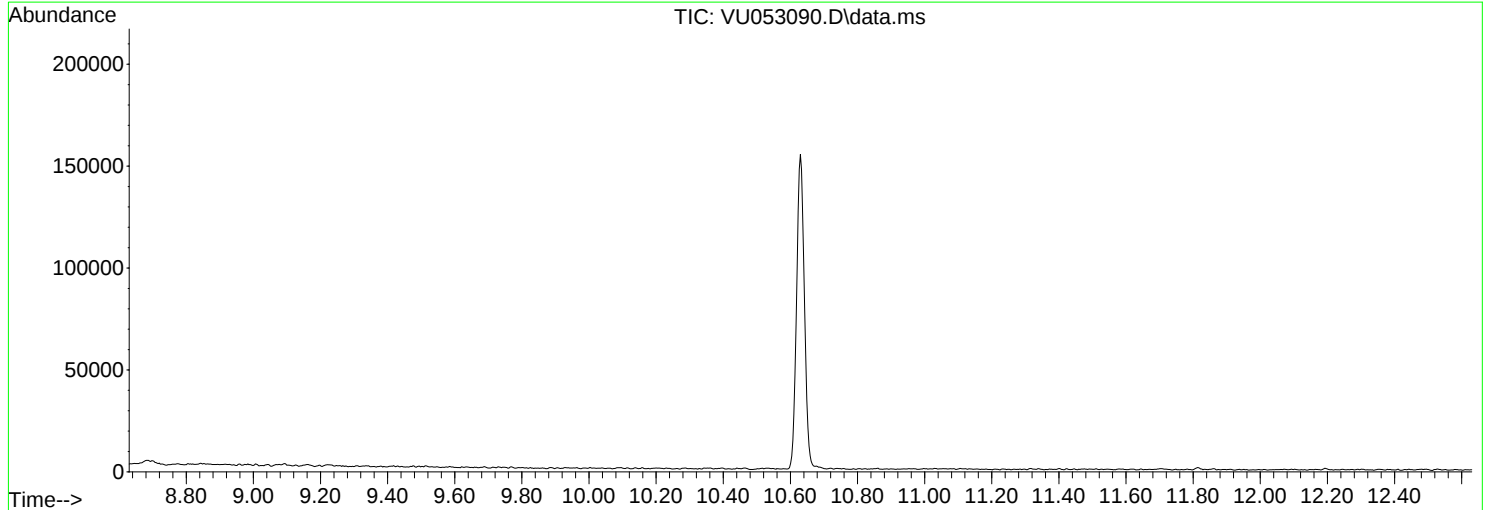

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2954

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	6107	PASS
75	95	30	80	52.5	17421	PASS
95	95	100	100	100.0	33184	PASS
96	95	5	9	6.5	2148	PASS
173	174	0.00	2	0.7	159	PASS
174	95	50	120	64.4	21387	PASS
175	174	5	9	7.0	1501	PASS
176	174	95	101	100.0	21395	PASS
177	176	5	9	6.1	1296	PASS

m/z	Abundance
36.00	745.0
38.00	241.0
41.10	110.0
43.10	132.0
44.00	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160

m/z	Abundance
35.10	185.0
36.10	997.0
37.10	1522.0
38.10	1249.0
39.10	557.0
43.00	100.0
44.00	354.0
45.00	266.0
47.00	397.0
48.00	203.0
49.10	1256.0
50.10	6010.0
51.10	1726.0
55.10	197.0
56.10	662.0
57.10	1001.0
60.00	266.0
61.10	1605.0
62.10	1390.0
63.10	1186.0
67.10	100.0
68.10	3478.0
69.10	3767.0
70.10	304.0
72.10	174.0
73.10	1549.0
74.10	6014.0
75.10	17432.0
76.10	1634.0
77.10	168.0
77.90	172.0
79.00	1314.0
80.00	415.0
81.00	1135.0
82.00	287.0
87.10	1404.0
88.00	1077.0
91.00	177.0
92.10	908.0
93.10	1362.0
94.10	3638.0
95.10	33096.0
96.10	2195.0
103.90	149.0
106.00	159.0
116.00	120.0
116.90	140.0
119.00	197.0
141.10	308.0
143.00	380.0
173.00	142.0
174.10	20808.0
175.10	1473.0
176.10	20496.0
177.00	1219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160

m/z	Abundance
35.10	160.0
36.10	981.0
37.10	1643.0
38.10	1395.0
39.10	659.0
40.10	109.0
43.10	116.0
44.00	381.0
45.00	253.0
47.00	417.0
48.00	201.0
49.10	1312.0
50.10	6348.0
51.10	1722.0
55.10	189.0
56.10	675.0
57.10	1160.0
60.00	263.0
61.10	1683.0
62.10	1357.0
63.10	1237.0
67.10	103.0
68.10	3604.0
69.10	3788.0
70.10	317.0
72.10	200.0
73.10	1579.0
74.10	6221.0
75.10	17880.0
76.10	1638.0
77.10	179.0
77.90	148.0
79.00	1360.0
80.00	442.0
81.00	1211.0
82.00	299.0
87.10	1460.0
88.10	1126.0
91.00	165.0
92.10	926.0
93.10	1523.0
94.10	3785.0
95.10	34232.0
96.10	2232.0
103.90	173.0
106.00	165.0
115.90	141.0
116.90	158.0
119.00	240.0
130.00	116.0
141.10	358.0
143.00	392.0
173.00	173.0
174.10	22080.0
175.10	1619.0
176.10	22088.0
177.00	1354.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160

m/z	Abundance
35.10	161.0
36.10	950.0
37.10	1510.0
38.10	1474.0
39.10	606.0
40.10	107.0
43.10	127.0
44.10	386.0
45.00	219.0
47.00	389.0
48.00	202.0
49.10	1310.0
50.10	5964.0
51.10	1634.0
55.10	157.0
56.10	636.0
57.10	1102.0
60.10	262.0
61.10	1561.0
62.10	1324.0
63.10	1212.0
67.20	100.0
68.10	3301.0
69.10	3439.0
70.10	308.0
72.10	207.0
73.10	1491.0
74.10	5798.0
75.10	16952.0
76.10	1500.0
77.10	164.0
79.00	1264.0
80.00	436.0
81.00	1191.0
82.10	283.0
87.10	1307.0
88.10	1151.0
91.00	164.0
92.10	858.0
93.10	1562.0
94.10	3683.0
95.10	32224.0
96.10	2018.0
103.90	173.0
106.00	166.0
115.90	139.0
116.90	155.0
119.00	231.0
127.90	104.0
130.00	118.0
141.10	351.0
143.00	350.0
172.90	161.0
174.10	21272.0
175.00	1411.0
176.10	21600.0
177.00	1316.0

Instrument :
MSVOA_U
ClientSampleId :
BFB160