


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021519\
 Data File : VU029486.D
 Acq On : 15 Feb 2019 09:45
 Operator : JC/SP
 Sample : BFB48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM021519WMA.M
 Title : VOC Analysis
 Last Update : Fri Feb 15 23:28:02 2019

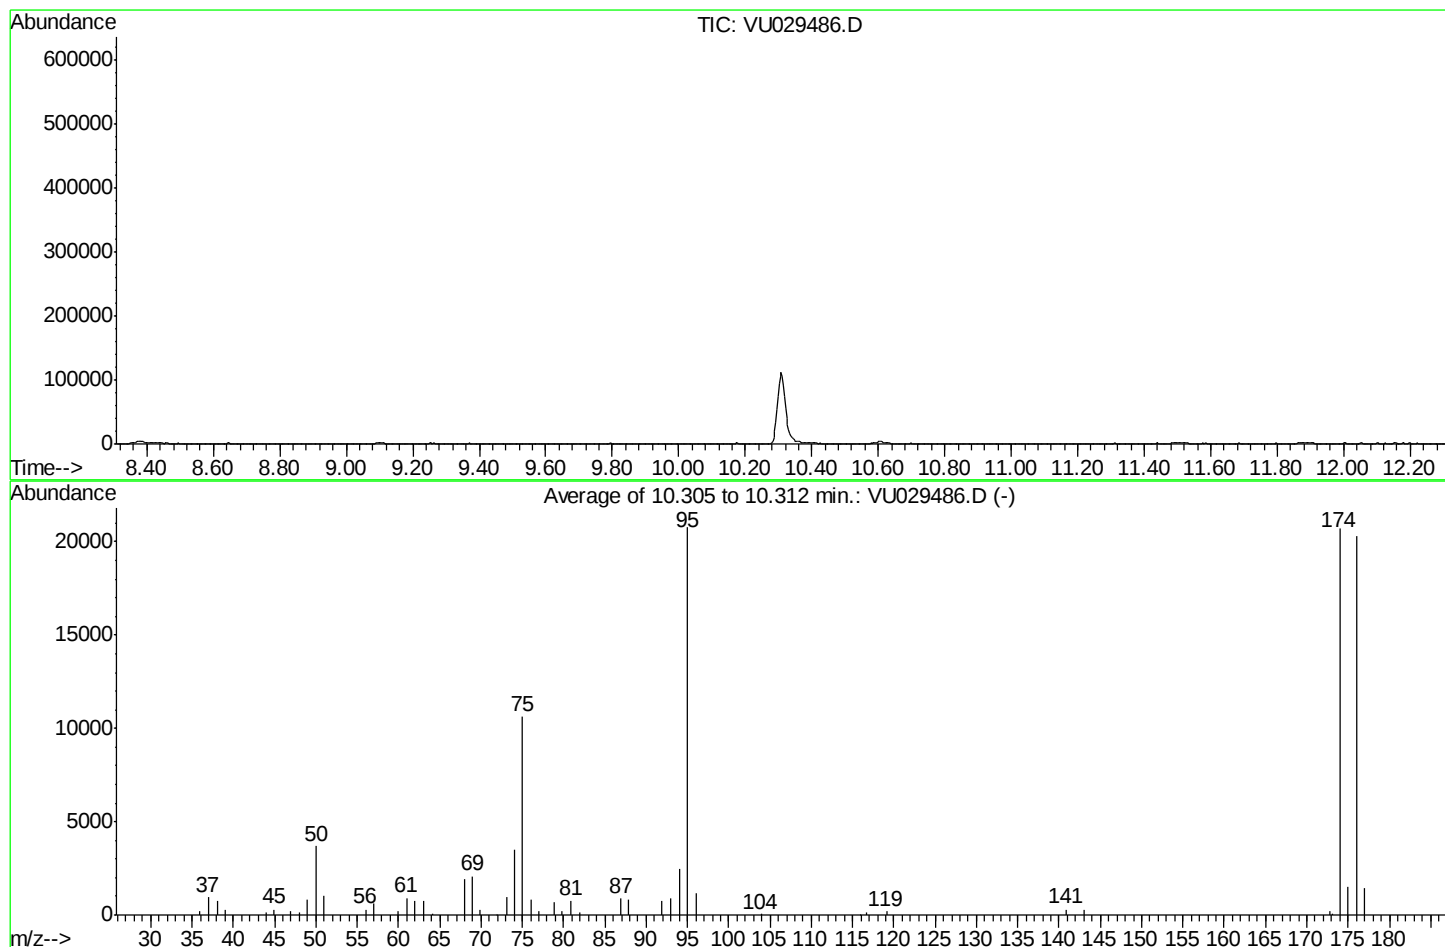

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	3701	PASS
75	95	30	80	51.1	10614	PASS
95	95	100	100	100.0	20773	PASS
96	95	5	9	5.7	1187	PASS
173	174	0.00	2	1.2	241	PASS
174	95	50	120	99.8	20733	PASS
175	174	5	9	7.2	1495	PASS
176	174	95	101	97.8	20274	PASS
177	176	5	9	7.0	1423	PASS

Scan 2855 (10.270 min): VU029486.D
BFB48

m/z	Abundance
39.80	137.0
41.10	109.0
43.90	452.0
207.00	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	219.0
37.00	1017.0
38.10	752.0
39.00	332.0
39.90	102.0
44.00	566.0
45.00	297.0
47.00	205.0
48.00	147.0
49.00	867.0
50.00	3714.0
50.90	927.0
56.10	288.0
56.90	639.0
60.00	188.0
61.00	972.0
62.00	754.0
63.00	771.0
64.10	146.0
68.00	1834.0
69.00	1965.0
69.90	216.0
71.90	100.0
73.00	984.0
74.00	3478.0
75.00	10286.0
76.00	829.0
77.00	229.0
78.90	762.0
79.80	196.0
80.90	769.0
82.00	186.0
86.90	718.0
87.90	708.0
91.90	739.0
93.00	905.0
94.00	2605.0
95.00	21024.0
96.00	1160.0
116.80	162.0
119.10	180.0
140.90	272.0
143.00	318.0
172.80	246.0
174.00	20512.0
175.00	1529.0
176.00	19408.0
176.90	1392.0
207.00	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	254.0
36.90	992.0
38.00	754.0
39.00	294.0
39.90	113.0
44.00	643.0
44.90	317.0
47.00	239.0
48.00	129.0
49.00	833.0
50.10	3755.0
50.90	1070.0
56.10	282.0
56.90	599.0
60.00	195.0
61.00	918.0
62.00	746.0
63.00	790.0
64.10	130.0
68.00	1955.0
69.00	2114.0
69.90	264.0
73.00	980.0
74.00	3607.0
75.00	10995.0
76.00	803.0
77.10	224.0
78.90	729.0
79.90	215.0
80.90	787.0
82.00	161.0
87.00	875.0
87.90	870.0
92.00	783.0
93.00	942.0
94.00	2546.0
95.00	21496.0
96.00	1206.0
116.80	149.0
119.10	180.0
140.90	291.0
143.00	288.0
172.70	256.0
174.00	21408.0
175.00	1543.0
176.00	20952.0
176.90	1514.0
207.10	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	253.0
36.90	864.0
38.00	711.0
39.00	275.0
40.00	128.0
44.00	605.0
44.90	265.0
46.90	250.0
47.90	153.0
49.00	766.0
50.00	3635.0
50.90	1130.0
55.90	262.0
57.00	565.0
60.00	191.0
61.00	804.0
62.00	766.0
63.00	698.0
68.00	1885.0
69.00	2112.0
69.90	268.0
73.10	905.0
74.10	3451.0
75.00	10562.0
76.00	758.0
77.10	132.0
78.90	669.0
79.90	203.0
80.90	716.0
81.90	124.0
87.00	1011.0
87.90	874.0
92.00	725.0
93.00	861.0
94.00	2242.0
95.00	19800.0
96.00	1197.0
103.90	124.0
115.90	107.0
116.70	118.0
119.10	170.0
140.90	307.0
143.00	247.0
172.70	222.0
173.10	182.0
174.00	20280.0
175.00	1413.0
176.00	20464.0
176.90	1363.0
207.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48