

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021522\
 Data File : VU047144.D
 Acq On : 15 Feb 2022 10:56
 Operator : SY/MD
 Sample : VU0215WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0215WBL01

Quant Time: Feb 17 08:01:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 15 03:17:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.118	96	54743	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	19807	0.934	ug/l	0.00
Spiked Amount 1.000			Recovery	=	93.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	21433	0.971	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021522\
Data File : VU047144.D
Acq On : 15 Feb 2022 10:56
Operator : SY/MD
Sample : VU0215WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0215WBL01

Quant Time: Feb 17 08:01:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 15 03:17:28 2022
Response via : Initial Calibration




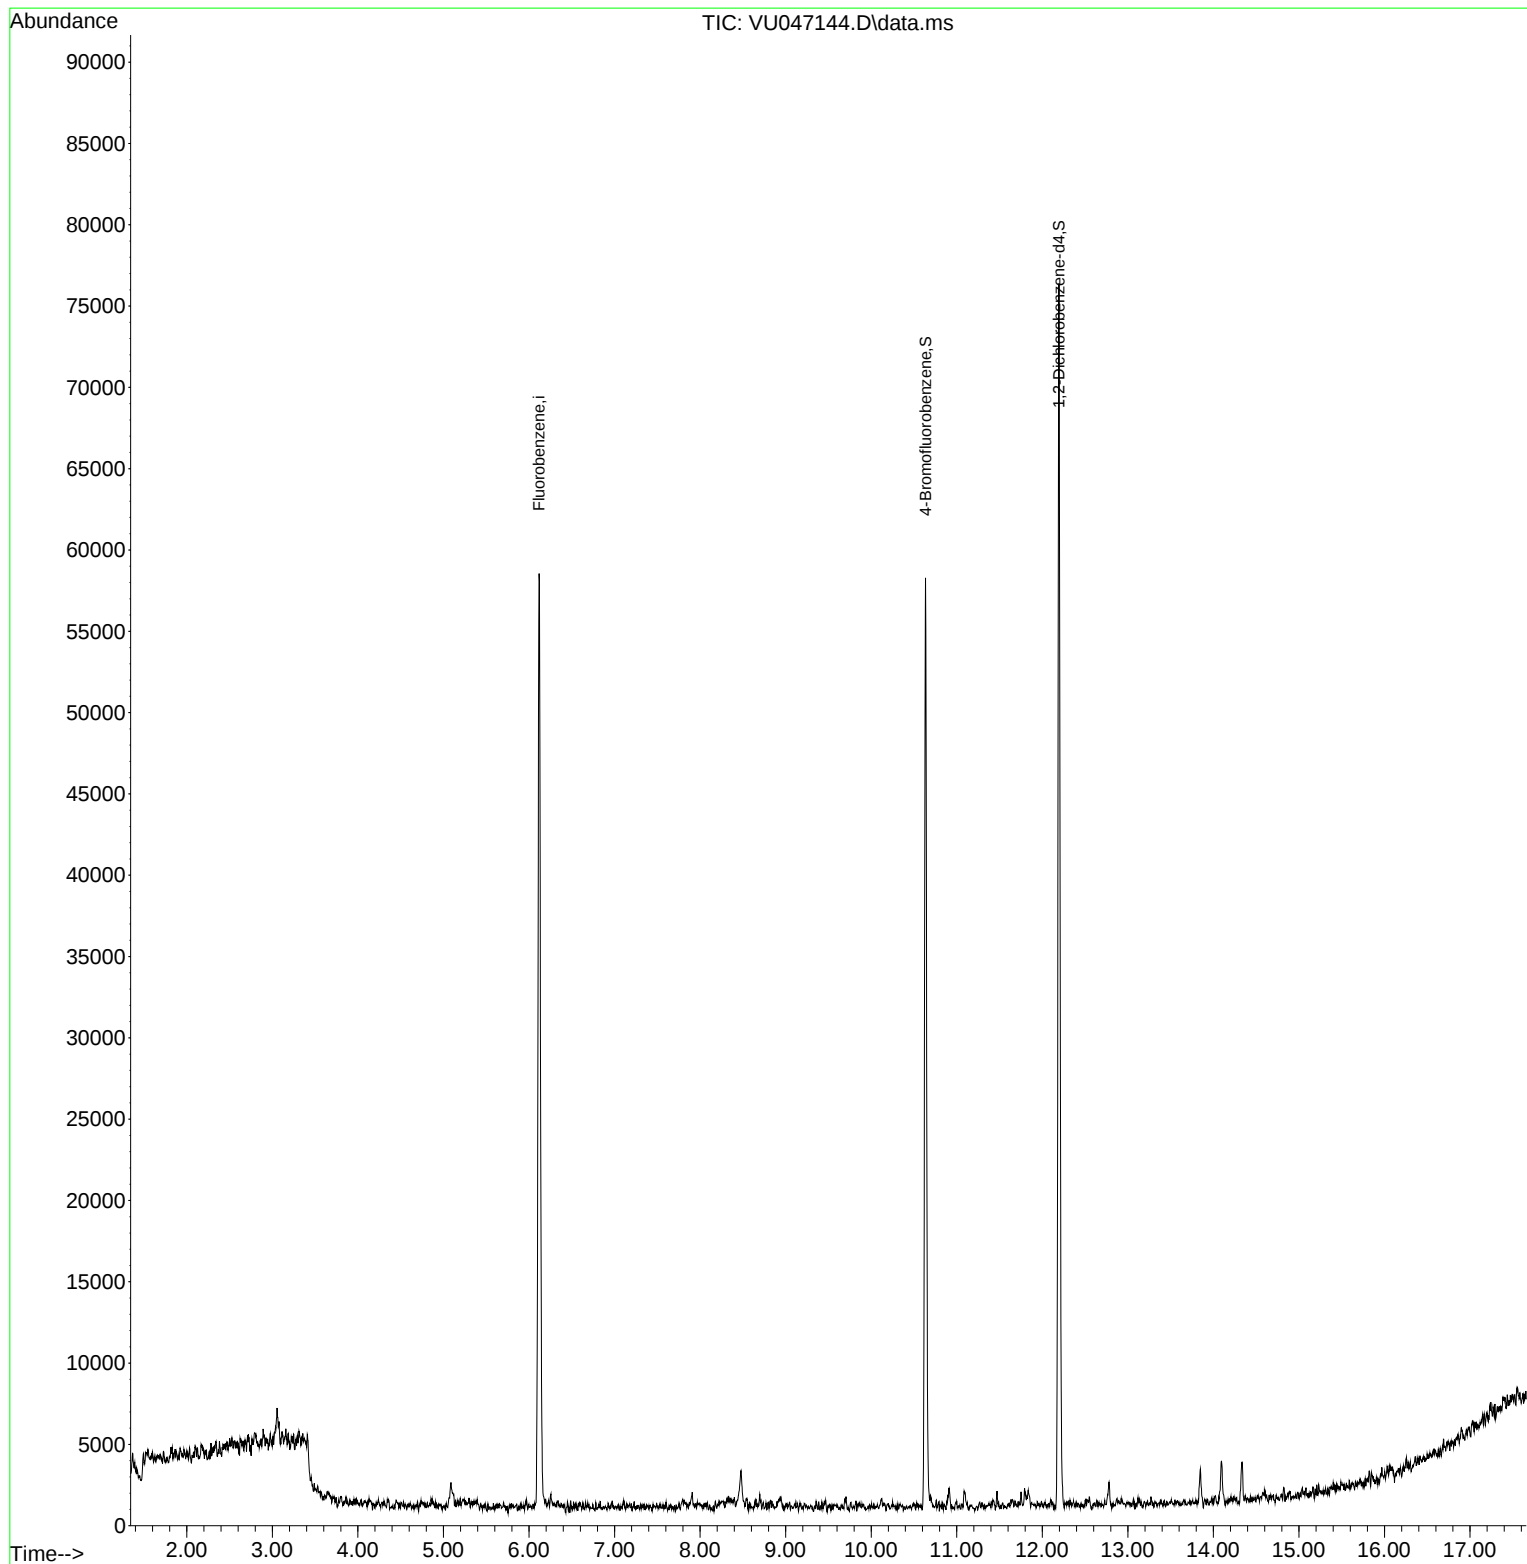


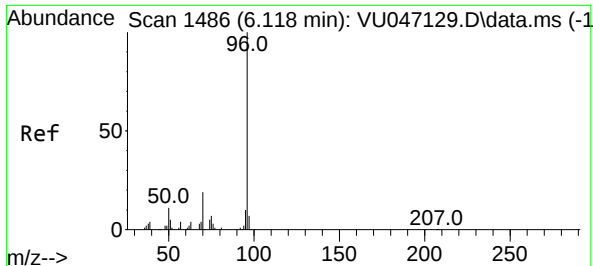

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.118 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VU047144.D
Acq: 15 Feb 2022 10:56




Instrument :
MSVOA_U
ClientSampleId :
VU0215WBL01


Tgt Ion: 96 Resp: 54743
Ion Ratio Lower Upper
96 100
70 20.0 16.8 25.2
95 8.9 7.3 10.9
97 6.7 0.0 0.0#

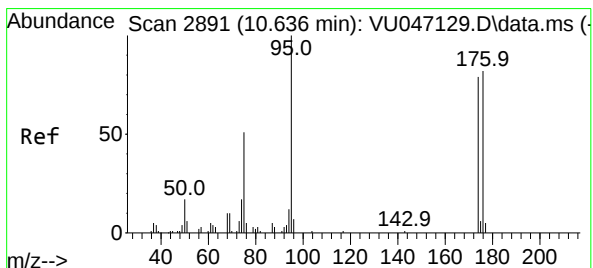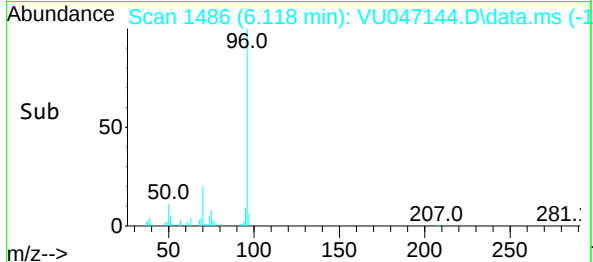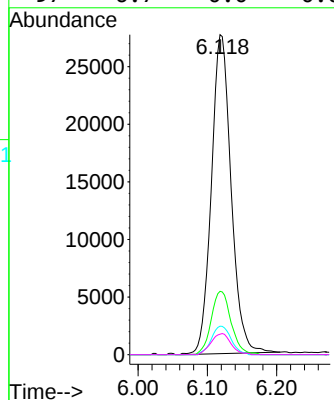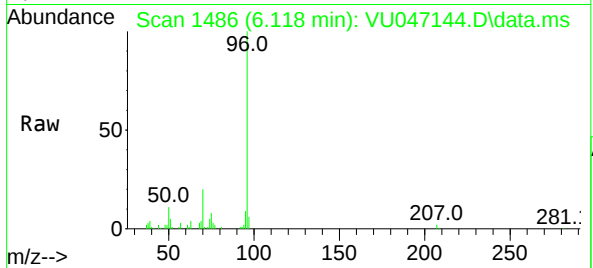

#57
4-Bromofluorobenzene
Concen: 0.934 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.000 min
Lab File: VU047144.D
Acq: 15 Feb 2022 10:56

Tgt Ion: 95 Resp: 19807
Ion Ratio Lower Upper
95 100
174 83.9 56.6 84.8
176 81.7 54.3 81.5#

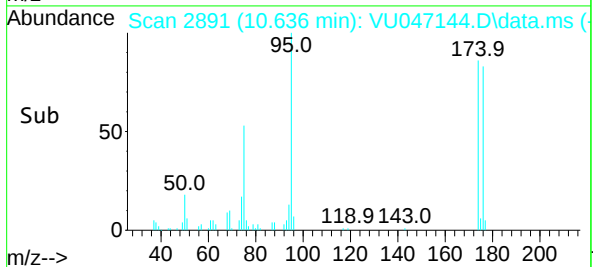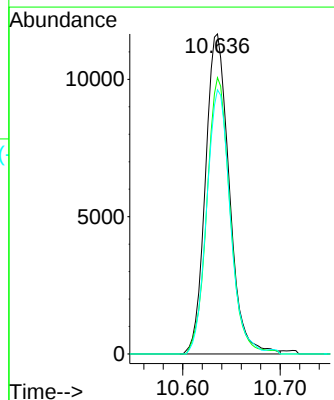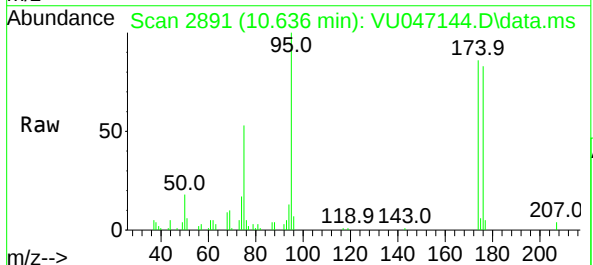

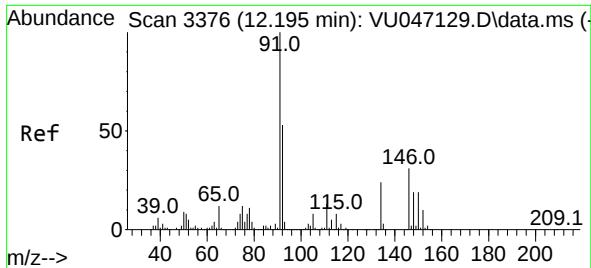

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.971 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VU047144.D
 Acq: 15 Feb 2022 10:56

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0215WBL01

Tgt Ion:	152	Resp:	21433
Ion Ratio	Lower	Upper	
152	100		
115	62.1	0.0	251.0
150	156.1	0.0	613.8

