
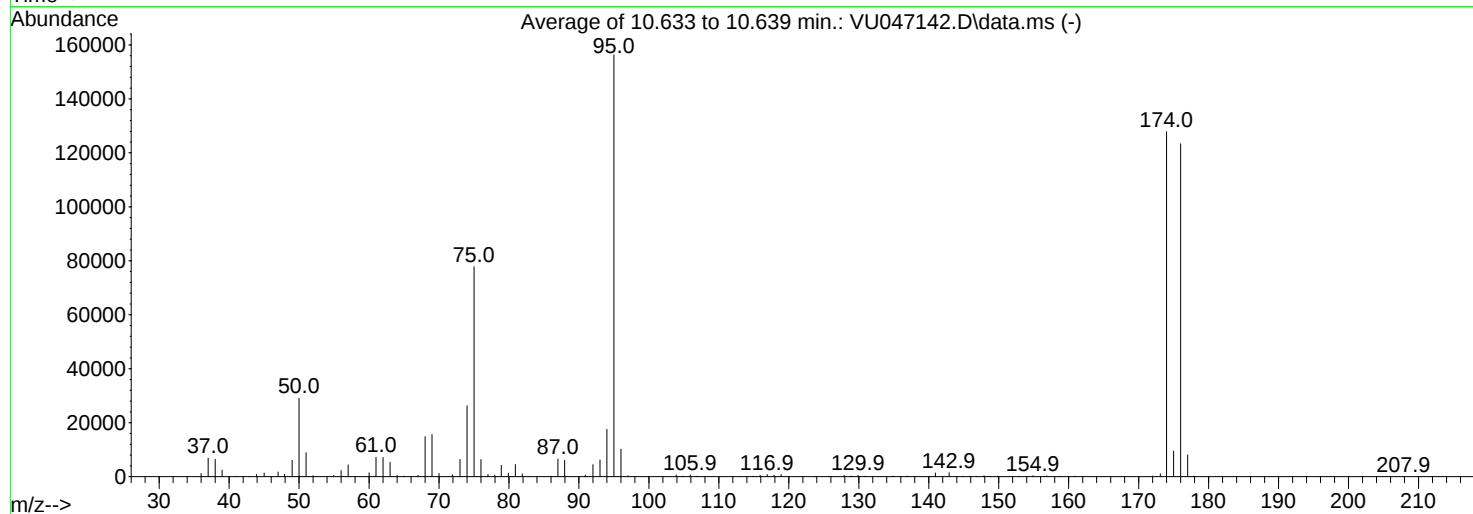


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021522\
 Data File : VU047142.D
 Acq On : 15 Feb 2022 09:23
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021422DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Tue Feb 15 03:17:28 2022

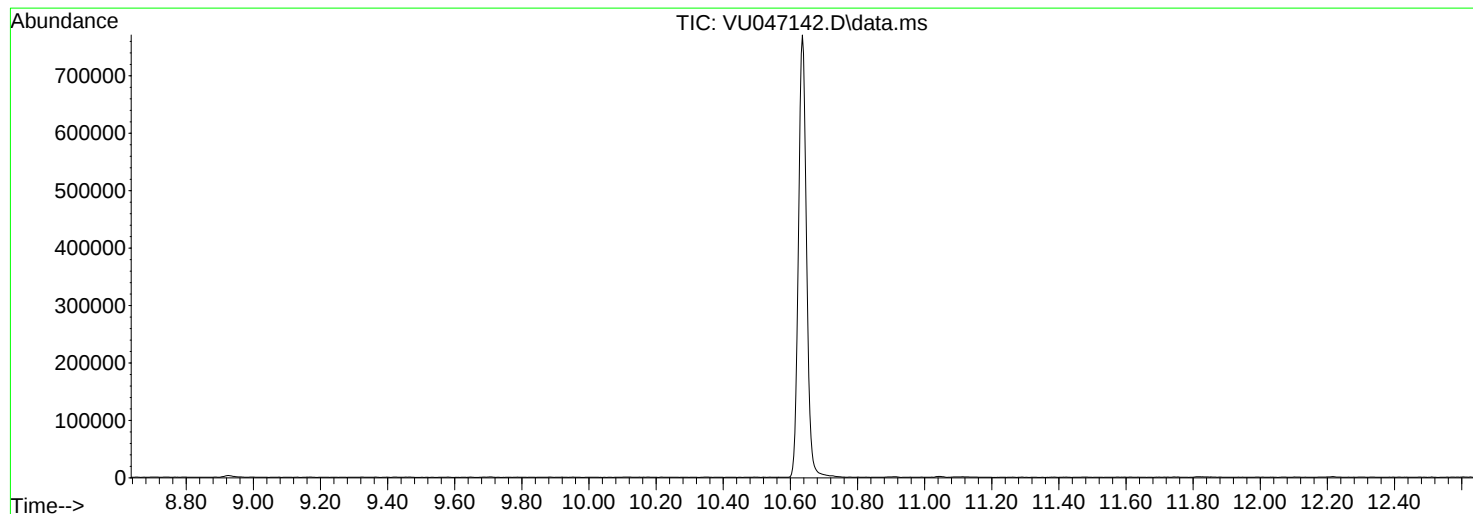

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	29013	PASS
75	95	30	60	49.8	77837	PASS
95	95	100	100	100.0	156331	PASS
96	95	5	9	6.5	10203	PASS
173	174	0.00	2	0.9	1095	PASS
174	95	50	100	81.8	127880	PASS
175	174	5	9	7.4	9468	PASS
176	174	95	101	96.4	123328	PASS
177	176	5	9	6.5	8076	PASS