

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021523\
 Data File : VU053109.D
 Acq On : 15 Feb 2023 12:56
 Operator : JC/MD
 Sample : VSTD00233
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Feb 16 00:45:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM021523.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 16 00:43:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	38594	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.346	117	33187	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	18860	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	47756	1.848	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.661	65	42267	1.746	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.639	67	59032	2.089	ug/L	0.00
8) Toluene-d8	7.830	98	129956	1.841	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.679	84	49545	2.050	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.598	62	47468	1.738	ug/L	98
6) Trichloroethene	6.489	95	55449	1.864	ug/L	98
9) 1,2-Dibromoethane	8.851	107	38656	2.101	ug/L #	95
12) 1,2,3-Trichloropropane	10.748	75	33767	2.123	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.907	75	7020	2.069	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021523\
Data File : VU053109.D
Acq On : 15 Feb 2023 12:56
Operator : JC/MD
Sample : VSTD00233
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Feb 16 00:45:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM021523.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 16 00:43:36 2023
Response via : Initial Calibration




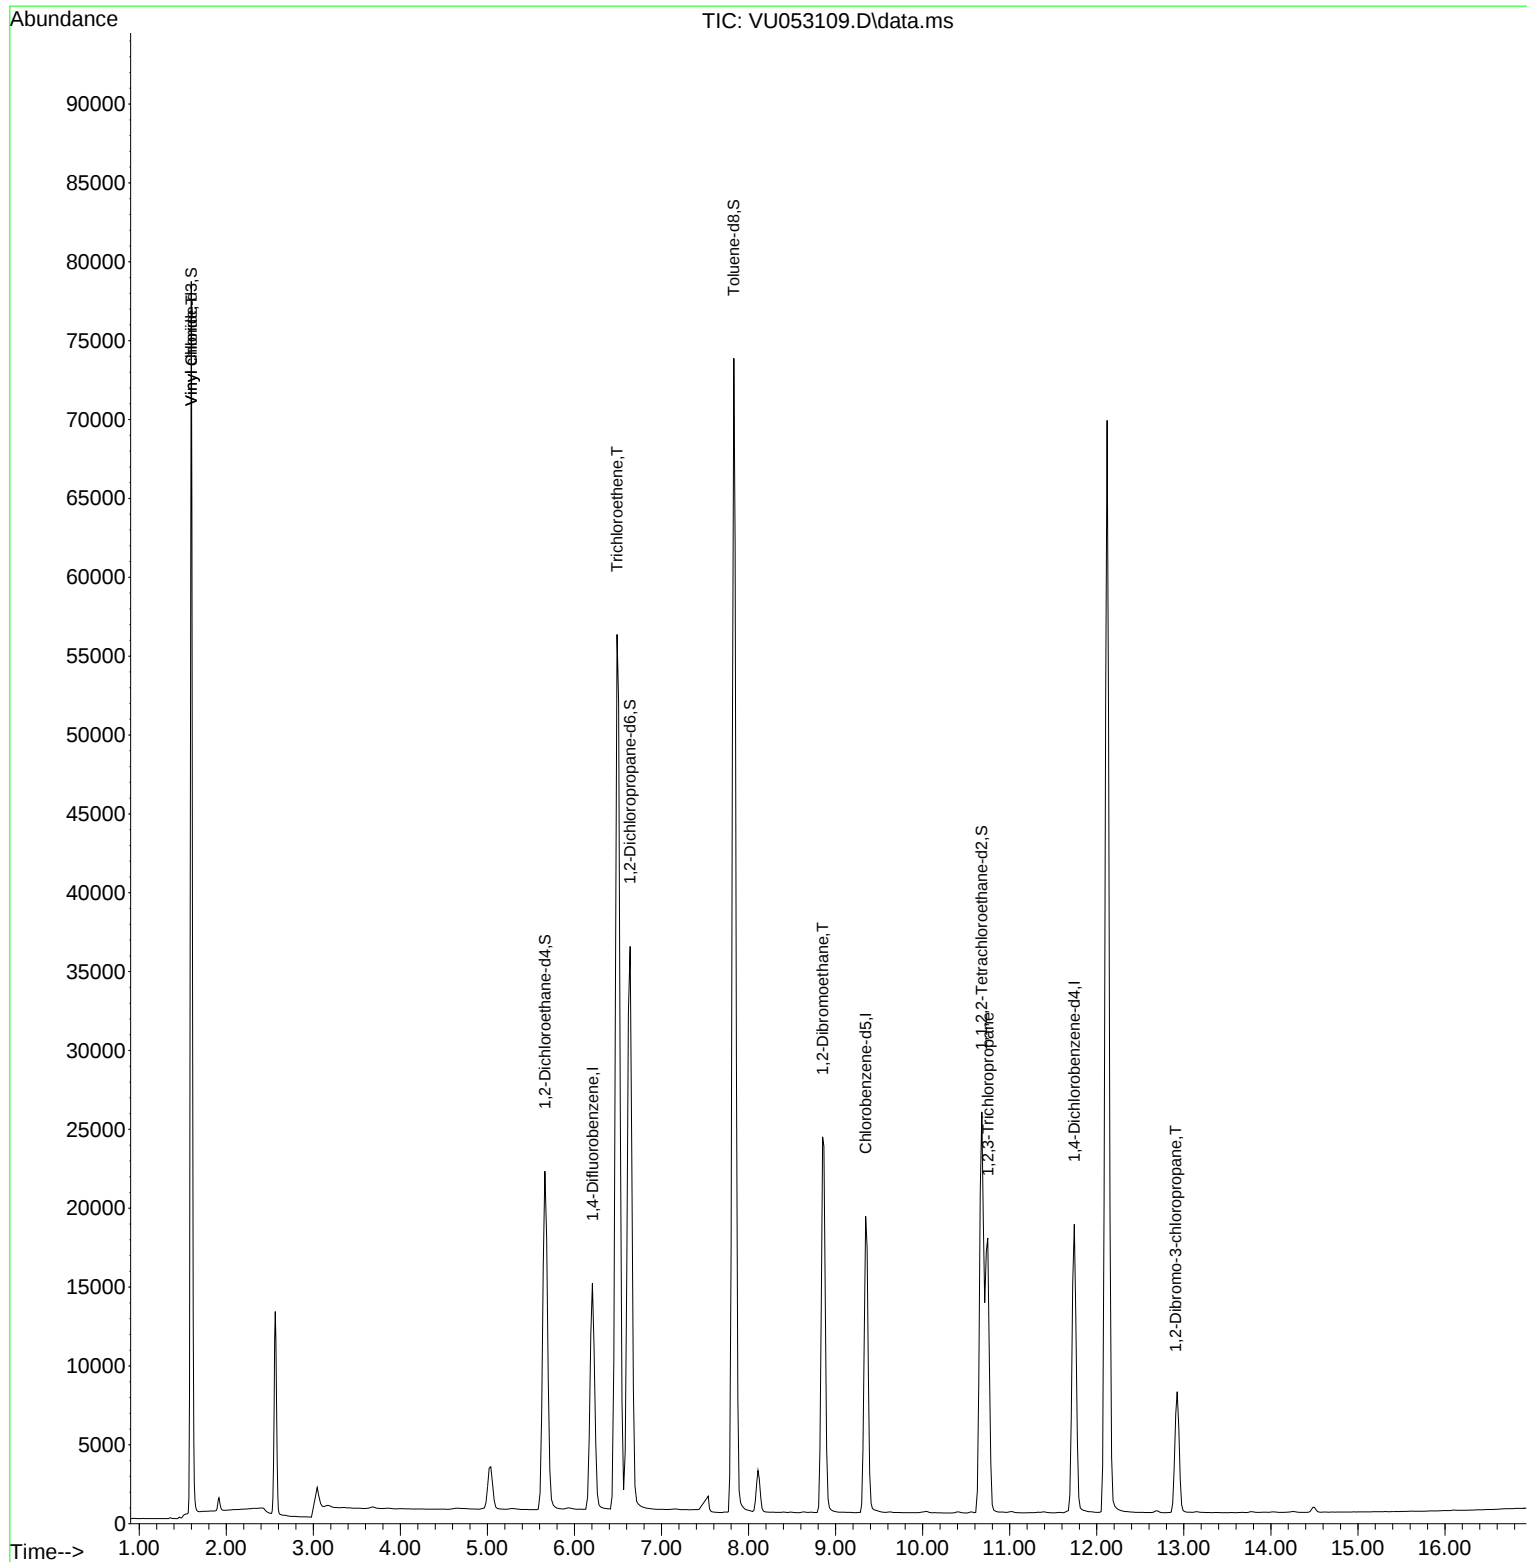


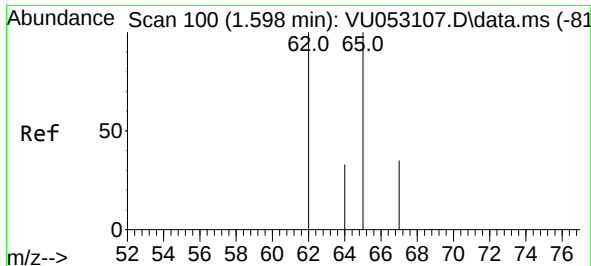

#3
 Vinyl chloride
 Concen: 1.738 ug/L
 RT: 1.598 min Scan# 100
 Delta R.T. 0.000 min
 Lab File: VU053109.D
 Acq: 15 Feb 2023 12:56




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion: 62 Resp: 47468
 Ion Ratio Lower Upper
 62 100
 64 32.8 23.7 43.9

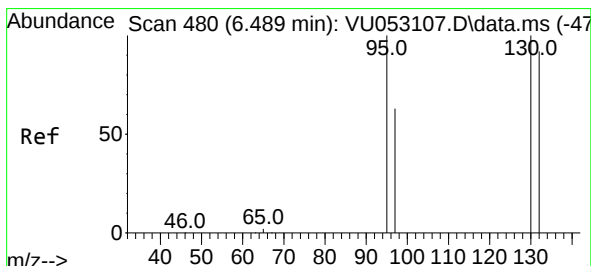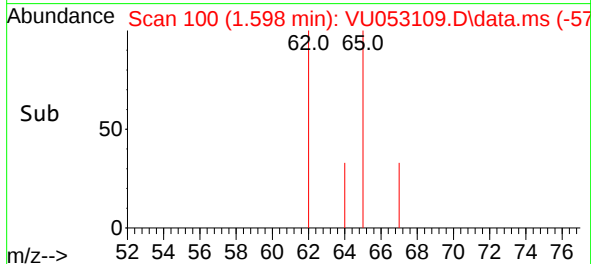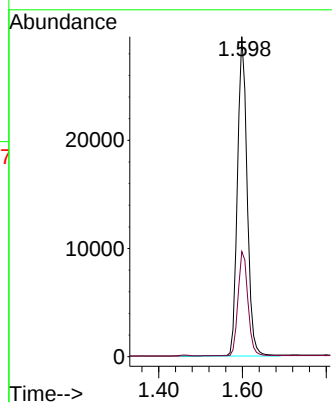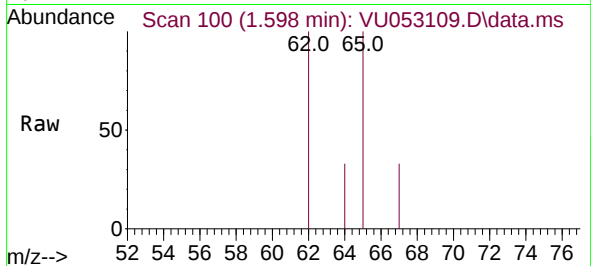

#6
 Trichloroethene
 Concen: 1.864 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. 0.000 min
 Lab File: VU053109.D
 Acq: 15 Feb 2023 12:56


Tgt Ion: 95 Resp: 55449
 Ion Ratio Lower Upper
 95 100
 97 63.7 44.7 83.1
 132 94.4 64.0 118.8
 130 101.0 69.0 128.2

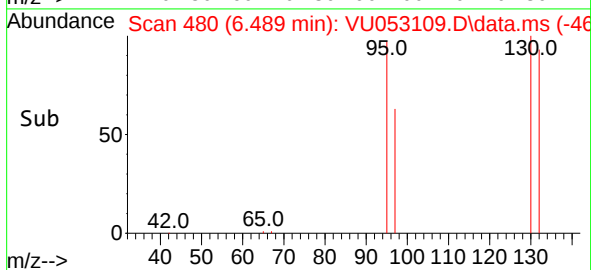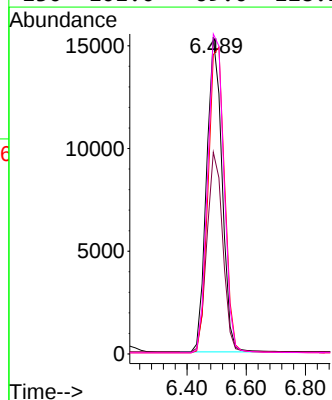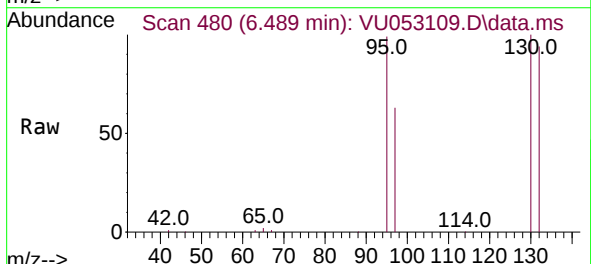



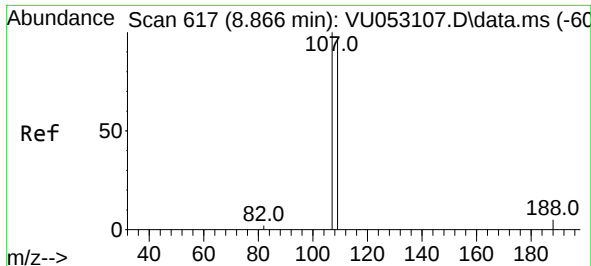


#9
1,2-Dibromoethane
Concen: 2.101 ug/L
RT: 8.851 min Scan# 617
Delta R.T. -0.015 min
Lab File: VU053109.D
Acq: 15 Feb 2023 12:56

Instrument :
MSVOA_U
ClientSampleId :



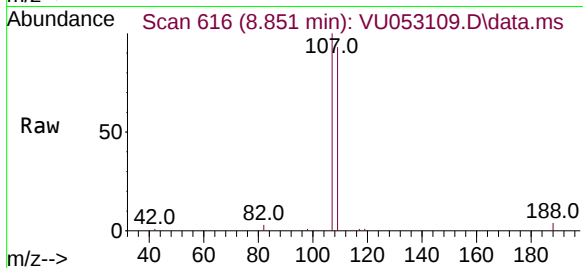



Tgt Ion:107 Resp: 38656
Ion Ratio Lower Upper
107 100
109 92.8 68.2 126.6
188 4.1 4.9 7.3#

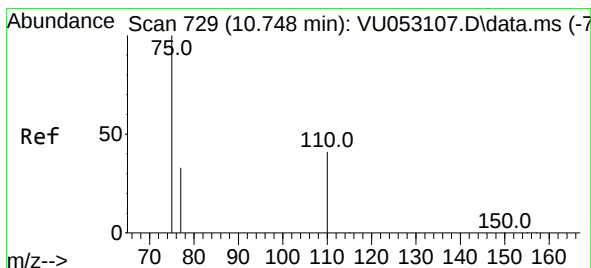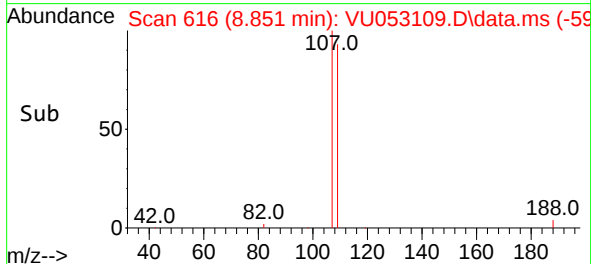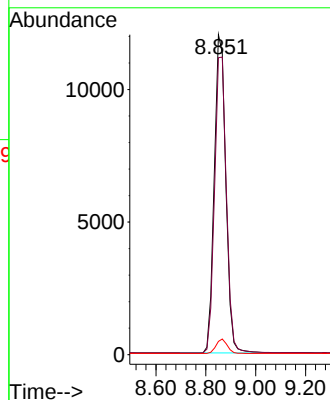

#12
1,2,3-Trichloropropane
Concen: 2.123 ug/L
RT: 10.748 min Scan# 729
Delta R.T. 0.000 min
Lab File: VU053109.D
Acq: 15 Feb 2023 12:56


Tgt Ion: 75 Resp: 33767
Ion Ratio Lower Upper
75 100
110 39.8 31.5 47.3
77 33.5 27.0 40.4

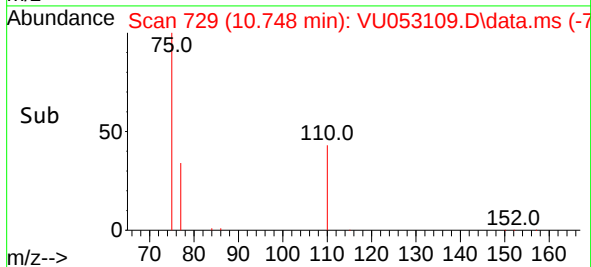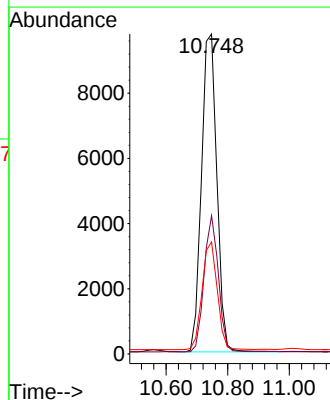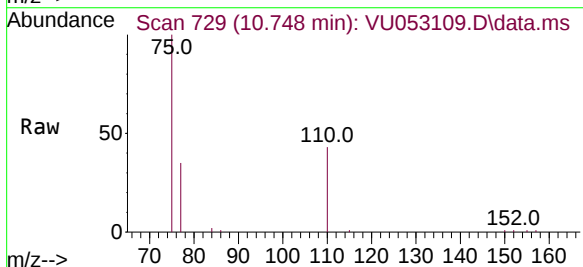

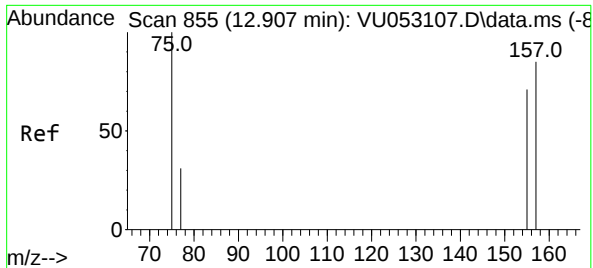

#13
 1,2-Dibromo-3-chloropropane
 Concen: 2.069 ug/L
 RT: 12.907 min Scan# 855
 Delta R.T. 0.000 min
 Lab File: VU053109.D
 Acq: 15 Feb 2023 12:56

Instrument :
 MSVOA_U
 ClientSampleId :

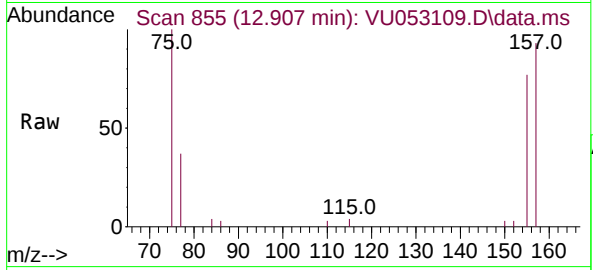

Tgt Ion:	75	Resp:	7020
Ion	Ratio	Lower	Upper
75	100		
157	92.8	67.2	100.8
155	77.3	58.2	87.2

