


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021523\
Data File : VU053104.D
Acq On : 15 Feb 2023 10:09
Operator : JC/MD
Sample : BFB012
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB012

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM021523.M
Title : TRACE VOA SOM01.0
Last Update : Thu Feb 16 00:50:34 2023

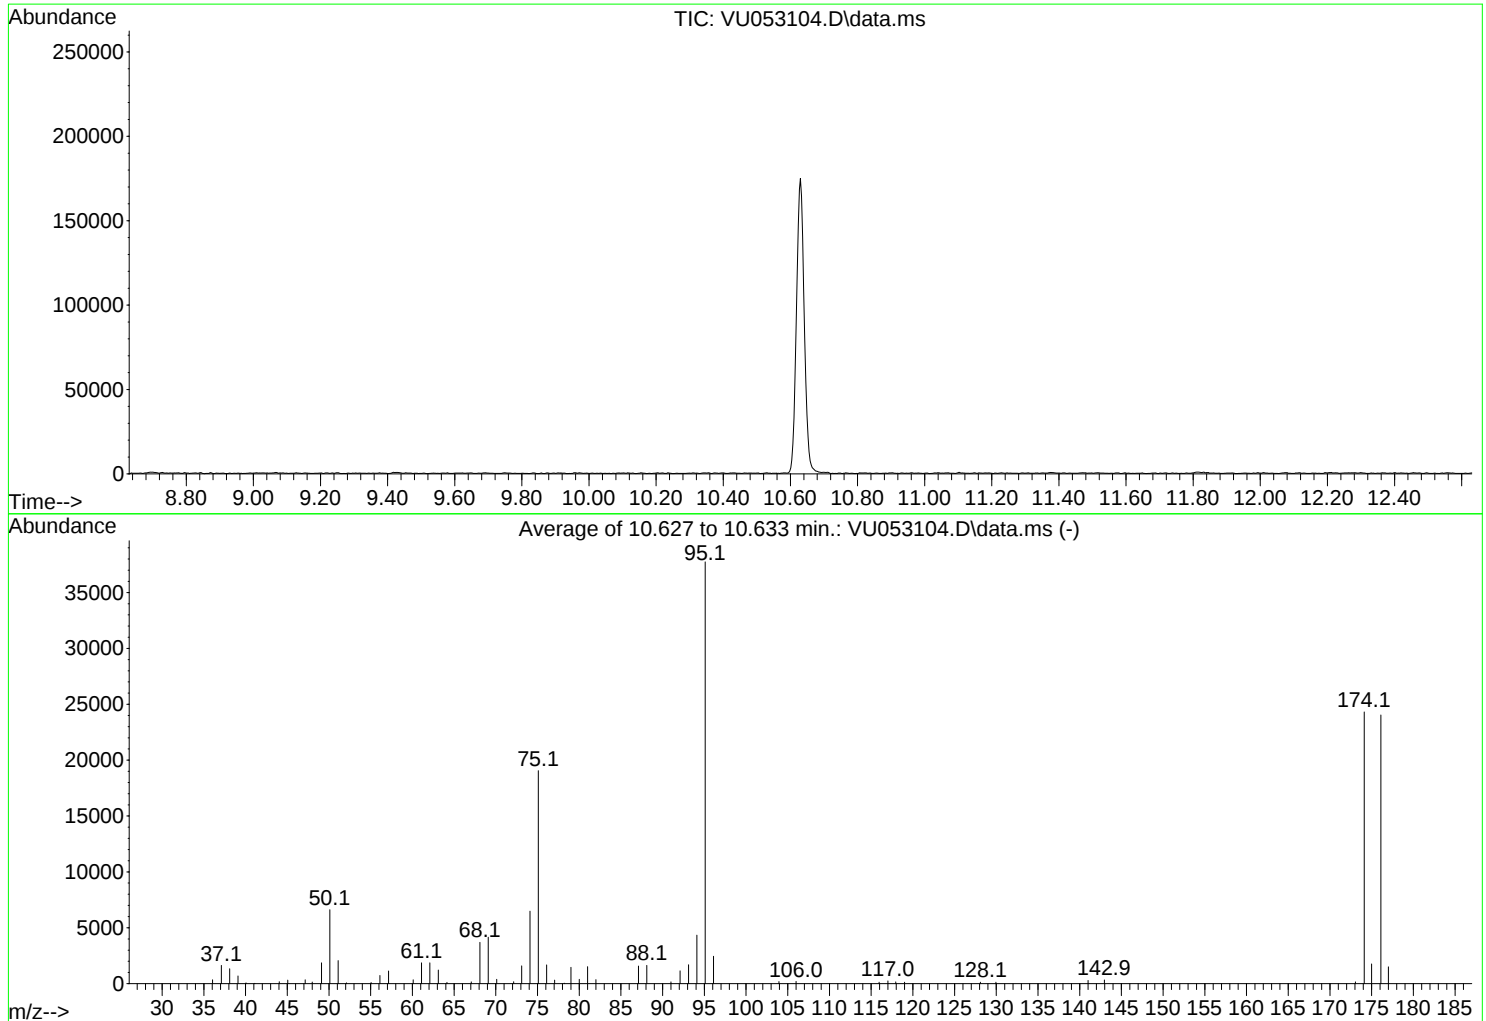

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2953

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	6610	PASS
75	95	30	80	50.5	19056	PASS
95	95	100	100	100.0	37747	PASS
96	95	5	9	6.5	2450	PASS
173	174	0.00	2	0.6	158	PASS
174	95	50	120	64.4	24312	PASS
175	174	5	9	7.2	1760	PASS
176	174	95	101	98.9	24037	PASS
177	176	5	9	6.3	1506	PASS

m/z	Abundance
43.10	155.0
44.00	315.0
55.00	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
36.00	270.0
37.10	1715.0
38.10	1254.0
39.10	679.0
41.10	109.0
44.10	513.0
45.00	300.0
47.20	314.0
48.00	151.0
49.10	1954.0
50.10	6713.0
51.10	2230.0
52.10	108.0
55.10	207.0
56.10	779.0
57.10	1137.0
60.10	349.0
61.10	1978.0
62.10	1994.0
63.10	1095.0
64.20	126.0
67.10	180.0
68.10	3830.0
69.10	4085.0
70.10	383.0
72.20	158.0
73.10	1542.0
74.10	6547.0
75.10	18664.0
76.10	1637.0
77.00	305.0
78.20	121.0
79.00	1506.0
80.00	353.0
81.00	1488.0
82.00	401.0
87.10	1571.0
88.10	1540.0
91.00	150.0
92.10	1151.0
93.10	1738.0
94.10	4476.0
95.10	37328.0
96.10	2521.0
104.00	173.0
106.00	183.0
115.90	156.0
117.00	211.0
118.00	160.0
119.00	117.0
128.10	126.0
130.00	111.0
141.00	298.0
142.90	332.0
173.00	135.0
174.10	23864.0
175.00	1786.0
176.10	23792.0
177.00	1504.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
36.00	345.0
37.10	1708.0
38.10	1379.0
39.10	722.0
40.00	112.0
44.10	498.0
45.00	319.0
47.10	328.0
48.00	150.0
49.10	1951.0
50.10	6814.0
51.10	2149.0
52.10	111.0
55.10	208.0
56.10	767.0
57.20	1150.0
60.10	353.0
61.10	1923.0
62.10	1912.0
63.10	1261.0
64.10	116.0
67.10	176.0
68.10	3766.0
69.10	4323.0
70.10	416.0
72.10	181.0
73.10	1618.0
74.10	6698.0
75.10	19696.0
76.10	1758.0
77.00	318.0
79.00	1473.0
80.00	390.0
81.00	1550.0
82.00	374.0
87.10	1639.0
88.10	1736.0
91.00	154.0
92.10	1205.0
93.10	1748.0
94.10	4490.0
95.10	39016.0
96.10	2528.0
103.90	206.0
106.00	201.0
115.90	131.0
117.00	248.0
117.90	169.0
119.00	126.0
128.10	137.0
129.90	137.0
141.00	293.0
142.90	332.0
173.10	167.0
174.10	25144.0
175.00	1811.0
176.10	24800.0
177.00	1571.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
36.10	403.0
37.10	1473.0
38.10	1378.0
39.10	678.0
40.10	122.0
44.10	448.0
45.10	330.0
47.10	399.0
48.00	140.0
49.10	1687.0
50.10	6302.0
51.10	1821.0
55.10	184.0
56.10	664.0
57.20	1092.0
60.10	346.0
61.10	1699.0
62.10	1698.0
63.10	1293.0
64.10	104.0
67.00	130.0
68.10	3499.0
69.10	4066.0
70.10	348.0
72.10	197.0
73.10	1619.0
74.10	6230.0
75.10	18808.0
76.10	1636.0
77.10	314.0
79.00	1382.0
80.00	421.0
81.00	1502.0
82.00	298.0
87.10	1511.0
88.10	1627.0
91.00	162.0
92.10	1087.0
93.10	1582.0
94.10	4034.0
95.10	36896.0
96.10	2301.0
103.90	177.0
106.00	216.0
116.00	105.0
117.00	273.0
117.90	127.0
119.00	138.0
128.10	123.0
129.90	127.0
141.00	283.0
143.00	311.0
173.10	173.0
174.10	23928.0
175.00	1682.0
176.10	23520.0
177.00	1444.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012