

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021524\
 Data File : VU057865.D
 Acq On : 15 Feb 2024 11:28
 Operator : MD/SY
 Sample : P1456-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA07

Quant Time: Feb 15 21:29:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Feb 15 21:28:35 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.242	114	194182	50.000	ug/L	0.00
28) Chlorobenzene-d5		9.412	117	180970	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.807	152	86900	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.595	65	94837	61.018	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	122.040%	
7) Chloroethane-d5		1.885	69	72801	60.378	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	120.760%	
11) 1,1-Dichloroethene-d2		2.557	63	126614	44.355	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.720%	
21) 2-Butanone-d5		4.611	46	103888	120.440	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	120.440%	
24) Chloroform-d		5.052	84	159303	57.779	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.560%	
26) 1,2-Dichloroethane-d4		5.692	65	110523	63.235	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	126.480%#	
32) Benzene-d6		5.717	84	332216	60.766	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	121.540%	
36) 1,2-Dichloropropane-d6		6.682	67	109821	63.609	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	127.220%#	
41) Toluene-d8		7.891	98	293079	59.131	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	118.260%	
43) trans-1,3-Dichloroprop...		8.174	79	49312	58.386	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	116.780%	
47) 2-Hexanone-d5		8.627	63	87046	123.519	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	123.520%	
56) 1,1,2,2-Tetrachloroeth...		10.753	84	145433	64.710	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	129.420%#	
66) 1,2-Dichlorobenzene-d4		12.190	152	104808	62.777	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	125.560%#	
Target Compounds							
13) Acetone		2.618	43	6313	5.697	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021524\
Data File : VU057865.D
Acq On : 15 Feb 2024 11:28
Operator : MD/SY
Sample : P1456-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA07

Quant Time: Feb 15 21:29:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 15 21:28:35 2024
Response via : Initial Calibration

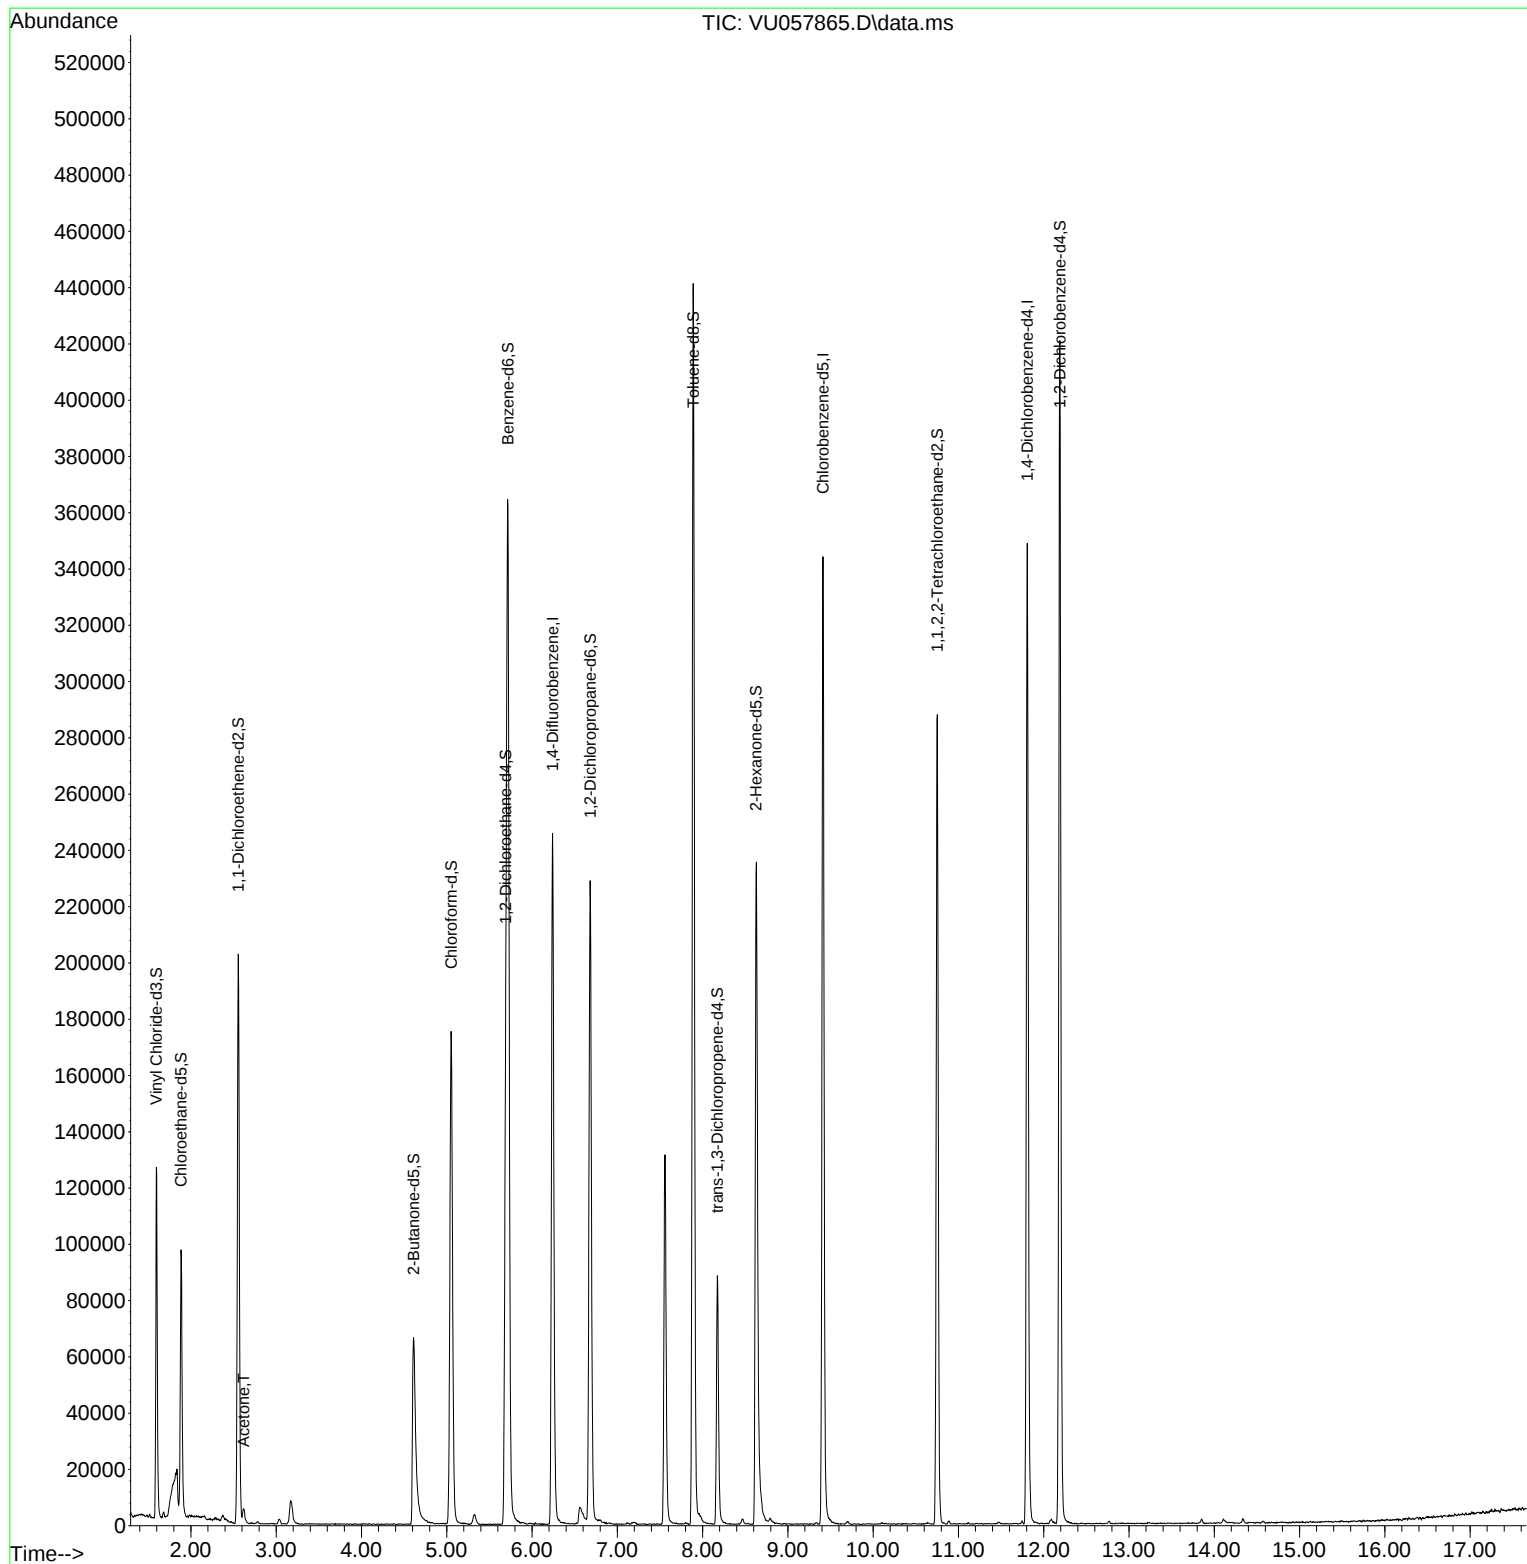

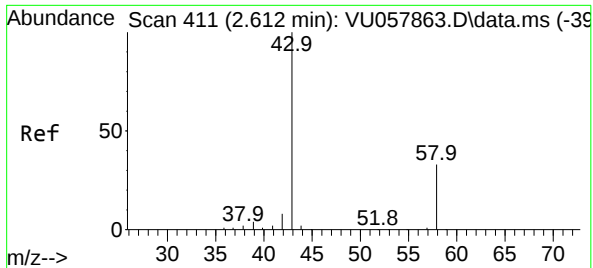

#13
 Acetone
 Concen: 5.697 ug/L
 RT: 2.618 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: VU057865.D
 Acq: 15 Feb 2024 11:28

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA07

Tgt Ion: 43 Resp: 6313
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 65.8

