


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021524\
Data File : VU057862.D
Acq On : 15 Feb 2024 09:08
Operator : MD/SY
Sample : BFB037
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB037

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Title : VOC Analysis
Last Update : Thu Feb 15 21:28:35 2024

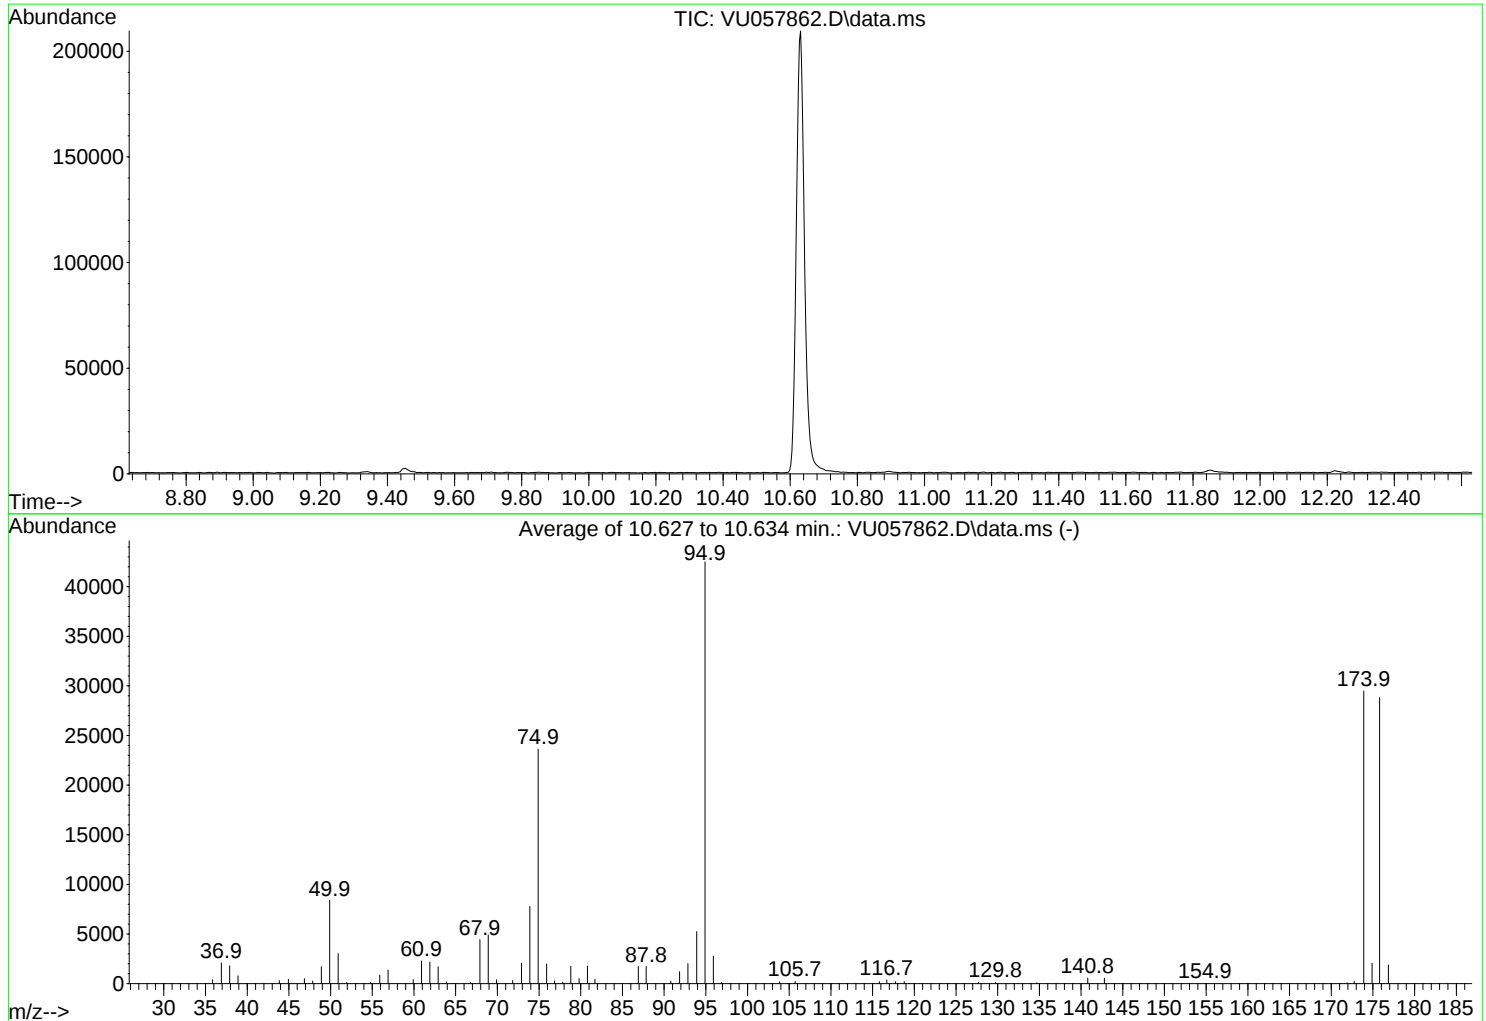

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	8380	PASS
75	95	30	80	55.6	23616	PASS
95	95	100	100	100.0	42501	PASS
96	95	5	9	6.5	2780	PASS
173	174	0.00	2	0.9	251	PASS
174	95	50	120	69.4	29485	PASS
175	174	5	9	7.0	2058	PASS
176	174	95	101	97.7	28821	PASS
177	176	5	9	6.5	1886	PASS

m/z	Abundance
39.90	213.0
43.80	442.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.90	384.0
36.90	2166.0
37.90	1956.0
38.90	714.0
39.80	234.0
44.00	729.0
44.90	392.0
46.80	522.0
47.90	234.0
48.90	1706.0
49.90	8556.0
50.90	3214.0
52.00	102.0
54.80	143.0
55.90	813.0
56.90	1368.0
59.90	411.0
60.90	2326.0
61.90	2284.0
62.90	1636.0
63.90	137.0
64.70	101.0
66.80	140.0
67.90	4454.0
68.90	4832.0
69.90	362.0
71.90	286.0
72.90	2170.0
73.90	7582.0
74.90	24472.0
75.90	2048.0
76.80	324.0
77.80	161.0
78.80	1938.0
79.80	477.0
80.80	1818.0
81.70	400.0
86.90	1798.0
87.80	1796.0
90.80	217.0
91.80	1278.0
92.80	2087.0
93.90	5364.0
94.90	42704.0
95.90	2835.0
96.90	121.0
103.80	148.0
104.80	108.0
105.70	199.0
115.80	214.0
116.70	368.0
117.70	217.0
118.80	199.0
127.70	117.0
129.70	132.0
134.70	117.0
140.80	548.0
142.80	566.0
154.90	102.0
171.90	149.0
172.80	215.0
173.90	28944.0
174.90	2085.0
175.80	28688.0
176.90	1945.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.80	389.0
36.90	2126.0
37.90	1810.0
38.90	821.0
39.80	228.0
43.90	780.0
44.90	453.0
46.90	541.0
47.70	182.0
48.00	188.0
48.90	1729.0
49.90	8621.0
50.90	3088.0
52.00	102.0
54.80	159.0
55.90	882.0
56.90	1421.0
59.90	412.0
60.90	2338.0
61.90	2283.0
62.90	1754.0
63.90	201.0
66.80	144.0
67.90	4565.0
68.90	5098.0
69.90	399.0
71.80	319.0
72.90	2101.0
73.90	8046.0
74.90	24352.0
75.90	2017.0
76.90	277.0
77.90	172.0
78.80	1805.0
79.80	555.0
80.80	1808.0
81.70	470.0
86.90	1804.0
87.90	1796.0
90.80	270.0
91.90	1254.0
92.90	2108.0
93.90	5352.0
94.90	43752.0
95.90	2882.0
96.90	130.0
103.90	174.0
105.70	241.0
115.80	222.0
116.70	398.0
117.80	206.0
118.80	197.0
127.70	111.0
129.70	135.0
134.70	105.0
140.80	600.0
142.80	558.0
171.90	116.0
172.70	284.0
173.90	30336.0
174.90	2089.0
175.80	29864.0
176.80	1921.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.80	372.0
36.90	1999.0
37.90	1613.0
38.90	819.0
39.80	208.0
43.90	735.0
45.00	440.0
46.90	447.0
47.80	196.0
48.90	1693.0
49.90	7963.0
50.90	2800.0
51.90	113.0
54.80	145.0
55.90	848.0
56.90	1315.0
59.90	409.0
60.90	2181.0
61.90	1987.0
62.90	1696.0
63.90	211.0
66.80	136.0
67.90	4298.0
68.90	4769.0
69.90	401.0
71.80	320.0
72.90	1939.0
73.90	7675.0
74.90	22024.0
75.90	1862.0
76.90	245.0
77.90	122.0
78.80	1545.0
79.80	534.0
80.80	1698.0
81.70	477.0
86.90	1553.0
87.90	1605.0
90.80	242.0
91.90	1090.0
92.90	1854.0
93.90	5008.0
94.90	41048.0
95.90	2622.0
96.90	101.0
103.90	197.0
105.70	251.0
115.80	209.0
116.70	341.0
117.80	177.0
118.80	167.0
127.70	122.0
129.80	132.0
140.80	562.0
142.80	529.0
172.70	253.0
173.90	29176.0
174.90	2001.0
175.80	27912.0
176.80	1792.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037