


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021619\
Data File : VU029498.D
Acq On : 15 Feb 2019 15:38
Operator : JC/SP
Sample : BFB49
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB49

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Feb 19 00:19:12 2019

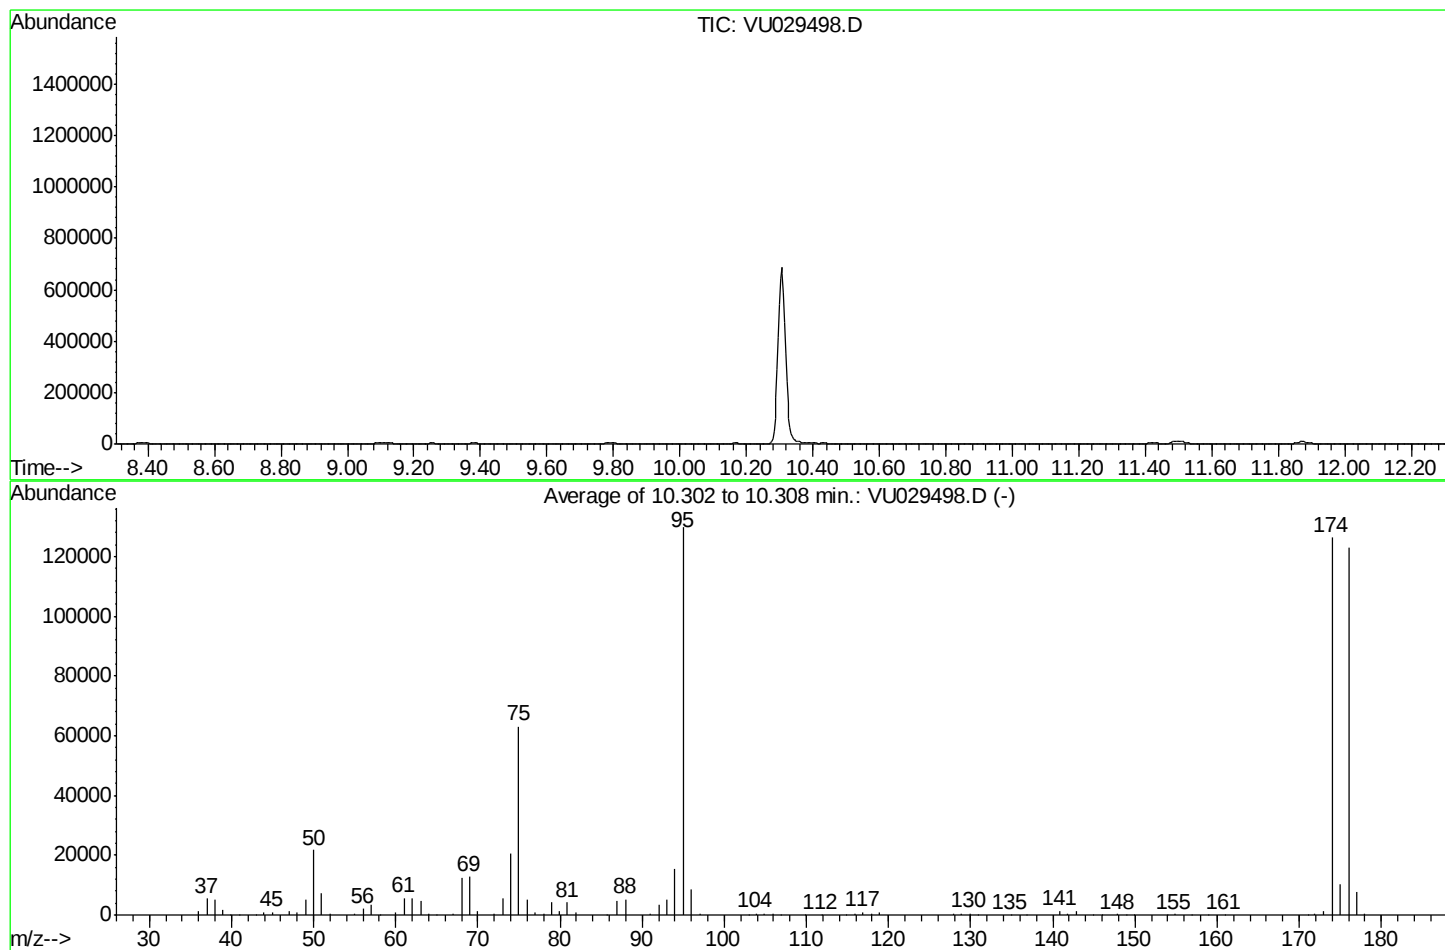

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	21832	PASS
75	95	30	80	48.7	63162	PASS
95	95	100	100	100.0	129778	PASS
96	95	5	9	6.6	8604	PASS
173	174	0.00	2	1.1	1394	PASS
174	95	50	120	97.4	126413	PASS
175	174	5	9	8.1	10202	PASS
176	174	95	101	97.3	122941	PASS
177	176	5	9	6.3	7705	PASS

Scan 2852 (10.260 min): VU029498.D
BFB49

m/z	Abundance
40.00	116.0
44.00	491.0
207.00	153.0
281.10	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	1118.0
37.00	5490.0
38.00	5337.0
39.00	1797.0
39.90	262.0
43.90	1223.0
45.00	971.0
47.00	1493.0
47.90	747.0
49.00	4874.0
50.00	21752.0
51.00	7225.0
52.00	348.0
55.00	432.0
56.00	2088.0
57.00	3538.0
60.00	1021.0
61.00	5409.0
62.00	5344.0
63.10	4504.0
63.90	453.0
65.00	117.0
67.00	318.0
68.00	11857.0
69.00	12712.0
70.00	1119.0
71.90	442.0
73.00	5659.0
74.00	20712.0
75.00	62976.0
76.10	4918.0
76.90	734.0
78.10	592.0
78.90	4267.0
79.90	1178.0
80.90	4094.0
81.90	917.0
85.80	148.0
87.00	4436.0
88.00	5070.0
90.90	553.0
92.00	3468.0
93.00	4927.0
94.00	15391.0
95.00	125840.0
96.00	8485.0
97.00	337.0
103.90	676.0
104.90	201.0
105.90	499.0
109.80	113.0
111.90	138.0
114.80	111.0
115.90	467.0
116.90	820.0
117.90	484.0
118.80	703.0
127.90	453.0
128.90	342.0
129.90	569.0
130.90	192.0
134.90	210.0
136.90	210.0
140.90	1429.0
141.80	299.0
142.90	1306.0
144.90	142.0
145.90	136.0
147.90	377.0
148.90	121.0
153.90	151.0
154.80	284.0
156.90	264.0
158.90	134.0
160.90	120.0
171.80	237.0
173.00	1330.0
174.00	119248.0
175.00	9827.0
176.00	116152.0
177.00	7618.0
177.90	226.0
207.10	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	1169.0
37.00	5580.0
38.00	5652.0
39.00	1920.0
39.90	274.0
41.00	115.0
43.00	128.0
43.90	1265.0
45.00	984.0
47.00	1560.0
47.90	769.0
49.00	5168.0
50.00	22504.0
51.00	7335.0
52.00	357.0
55.00	412.0
56.00	2118.0
57.00	3606.0
60.00	1060.0
61.00	5838.0
62.00	5545.0
63.10	4770.0
63.90	465.0
65.00	127.0
67.00	312.0
68.00	12943.0
69.00	13199.0
70.00	1151.0
71.90	524.0
73.00	5960.0
74.00	21384.0
75.00	65208.0
76.00	5117.0
76.90	804.0
78.00	632.0
78.90	4558.0
79.90	1209.0
80.90	4291.0
81.90	1089.0
85.80	153.0
87.00	4671.0
88.00	5508.0
90.90	617.0
92.00	3597.0
93.00	5100.0
94.00	15746.0
95.00	134016.0
96.00	8839.0
97.00	265.0
103.00	111.0
103.90	697.0
104.90	273.0
105.90	541.0
109.80	148.0
111.90	168.0
114.80	121.0
115.90	486.0
116.90	979.0
117.90	523.0
118.80	694.0
127.90	473.0
128.80	345.0
129.90	594.0
130.90	184.0
134.90	195.0
136.80	240.0
140.90	1424.0
141.80	330.0
142.90	1377.0
144.90	154.0
145.90	159.0
147.90	367.0
149.90	115.0
153.80	158.0
154.90	324.0
156.80	222.0
158.90	161.0
160.90	122.0
171.90	310.0
172.90	1440.0
174.00	130592.0
175.00	10652.0
176.00	127224.0
177.00	7928.0
177.90	279.0
207.10	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	1095.0
37.00	5084.0
38.00	5091.0
39.00	1837.0
39.90	247.0
41.00	107.0
43.00	169.0
43.90	1269.0
45.00	898.0
47.10	1391.0
48.00	745.0
49.00	4898.0
50.00	21240.0
51.00	6807.0
52.00	311.0
55.00	351.0
56.00	2020.0
57.00	3330.0
58.10	107.0
59.90	955.0
61.00	5766.0
62.00	5338.0
63.00	4590.0
64.00	433.0
65.00	108.0
67.00	302.0
68.00	12566.0
69.00	12538.0
70.00	1056.0
72.00	624.0
73.00	5614.0
74.00	20184.0
75.00	61304.0
76.00	4936.0
77.00	844.0
78.00	572.0
78.90	4323.0
79.90	1162.0
80.90	4146.0
81.90	1047.0
85.70	120.0
86.90	4562.0
87.90	5489.0
90.90	536.0
92.00	3444.0
93.00	5073.0
94.00	14629.0
95.00	129480.0
96.00	8488.0
97.00	207.0
103.00	112.0
103.90	593.0
104.90	278.0
105.90	598.0
106.80	113.0
109.80	157.0
111.80	160.0
114.80	115.0
115.90	491.0
116.90	955.0
117.90	479.0
118.80	670.0
127.90	469.0
128.80	340.0
129.90	577.0
130.90	134.0
134.90	174.0
136.80	232.0
140.90	1354.0
141.80	298.0
142.90	1330.0
144.90	173.0
146.00	248.0
147.90	346.0
149.80	143.0
153.80	107.0
154.90	340.0
156.80	202.0
158.90	180.0
160.90	124.0
171.10	103.0
171.90	293.0
173.00	1412.0
174.00	129400.0
175.00	10127.0
176.00	125448.0
177.00	7569.0
177.90	280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49