
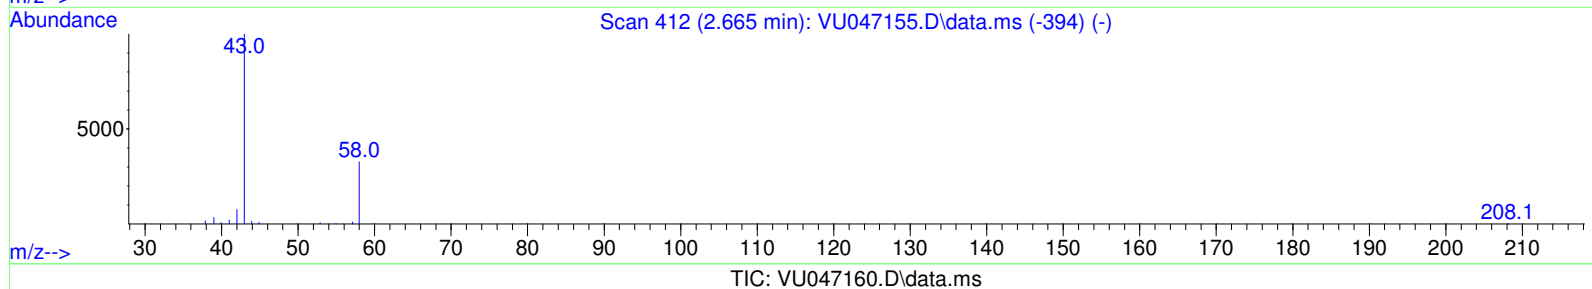
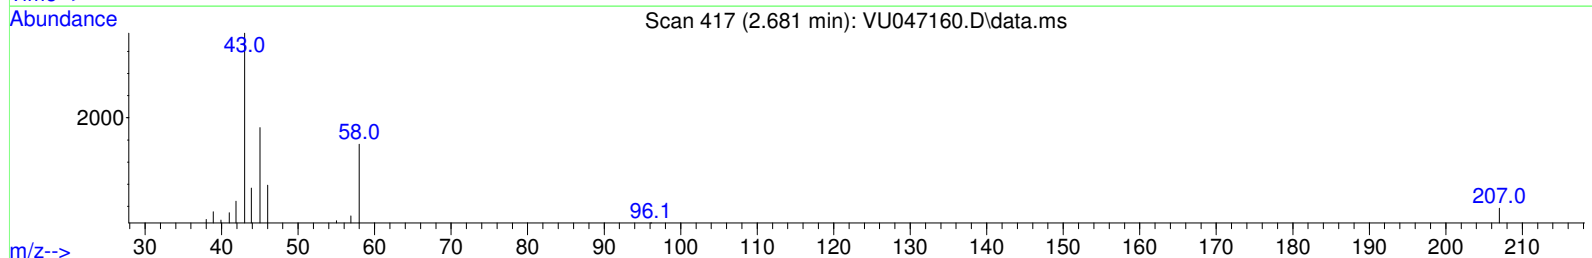


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047160.D
Acq On : 16 Feb 2022 14:51
Operator : SY/MD
Sample : N1545-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 16 15:12:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 16 13:52:04 2022
Response via : Initial Calibration

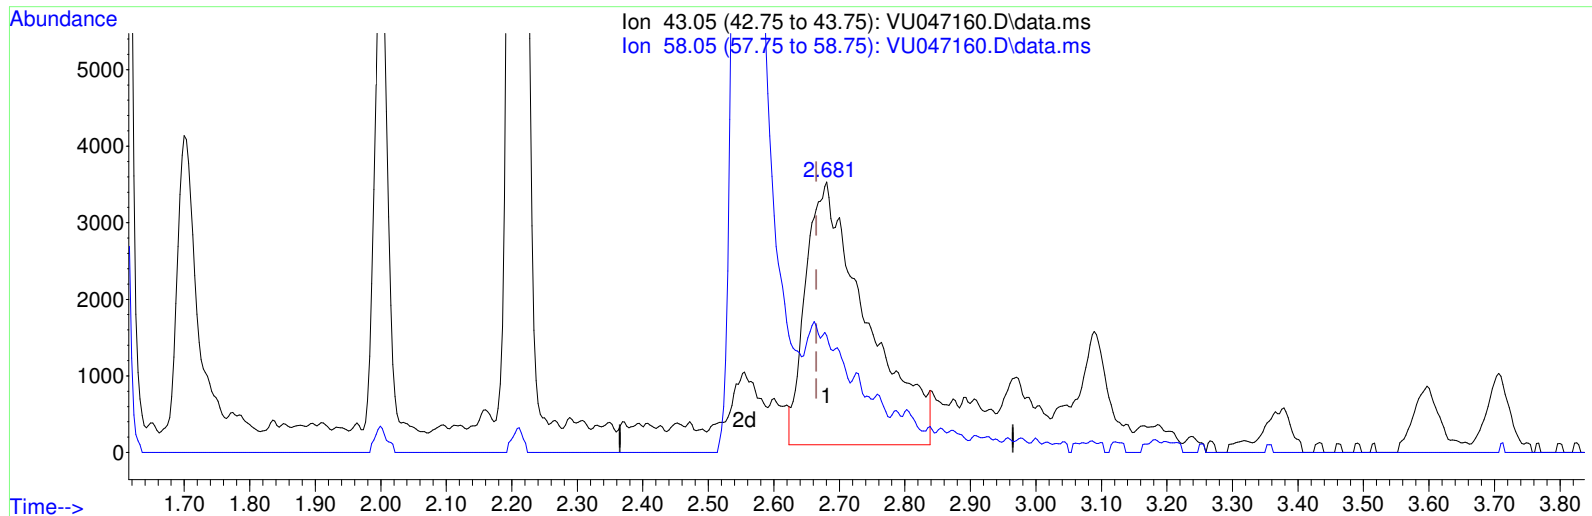

(13) Acetone (T)

2.681min (+ 0.016) 12.13 ug/L m

response 22098

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	0.00
0.00	0.00	0.00
0.00	0.00	0.00