

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
 Data File : VU047188.D
 Acq On : 17 Feb 2022 04:04
 Operator : SY/MD
 Sample : N1558-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M69

Quant Time: Feb 17 04:54:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 13:52:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	165610	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	167906	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	95260	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	59932	4.285	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.600%
7) Chloroethane-d5	1.919	69	50252	4.533	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.575	65	23478	4.059	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.200%
20) 2-Butanone-d5	4.639	46	181394	54.259	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.520%
24) Chloroform-d	5.070	84	108294	4.661	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	5.706	65	60724	4.700	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.732	84	223426	4.763	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.200%
36) 1,2-Dichloropropane-d6	6.694	67	71706	4.803	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.899	98	212638	4.633	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
43) trans-1,3-Dichloroprop...	8.182	79	28065	4.147	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.000%
46) 2-Hexanone-d5	8.636	63	155986	43.778	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.560%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	59300	4.371	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	82563	4.831	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.600%
Target Compounds					Qvalue	
13) Acetone	2.662	43	6738	4.026	ug/L	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047188.D
Acq On : 17 Feb 2022 04:04
Operator : SY/MD
Sample : N1558-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M69

Quant Time: Feb 17 04:54:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 16 13:52:04 2022
Response via : Initial Calibration

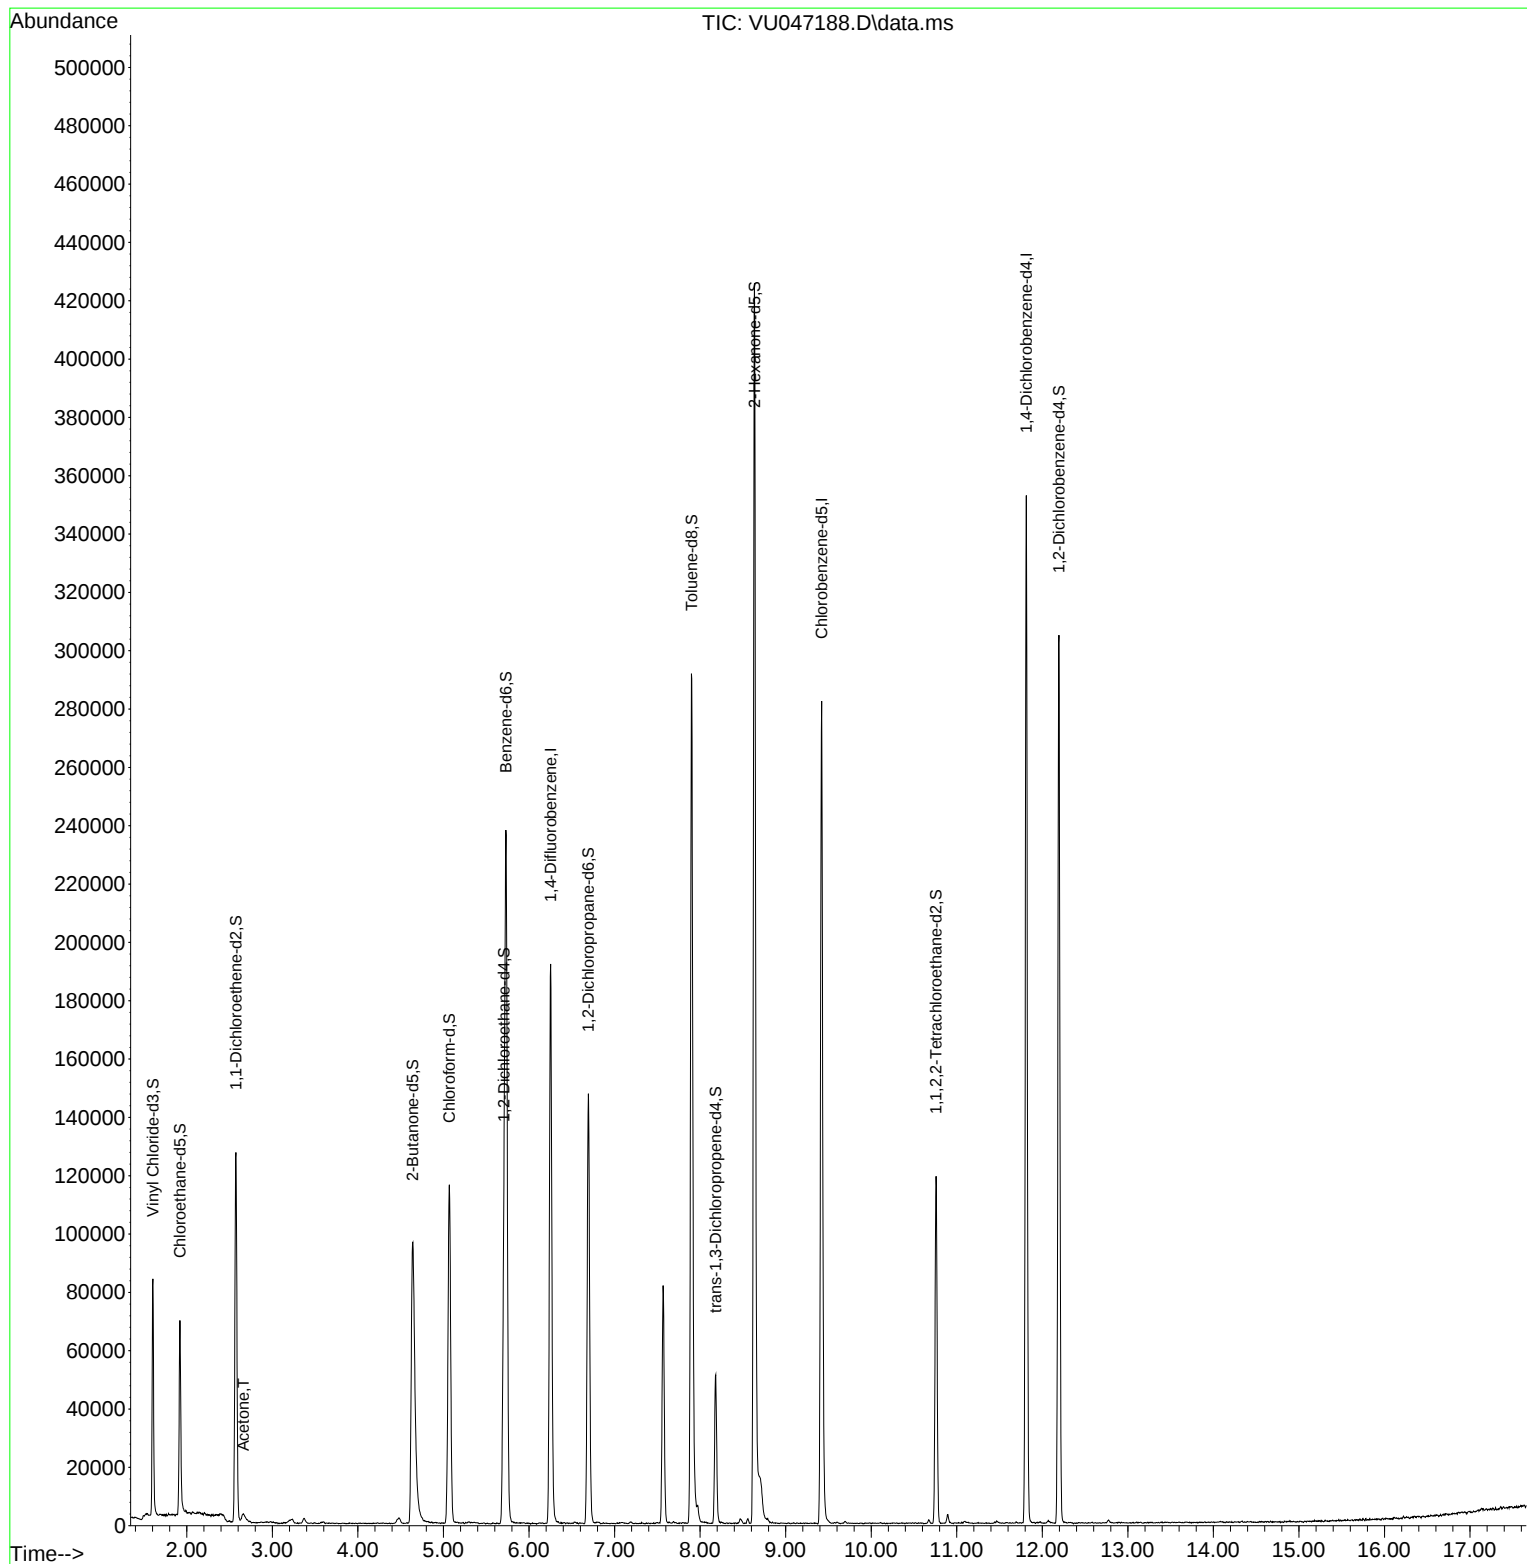

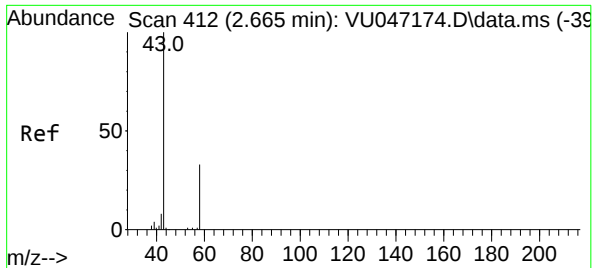

#13
 Acetone
 Concen: 4.026 ug/L
 RT: 2.662 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU047188.D
 Acq: 17 Feb 2022 04:04

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M69

Tgt Ion: 43 Resp: 6738
 Ion Ratio Lower Upper
 43 100
 58 8.1 0.0 71.6

