

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
 Data File : VU047173.D
 Acq On : 16 Feb 2022 20:03
 Operator : SY/MD
 Sample : N1558-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M64

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	88596	103700	12.51%	1.558%
2	1.919	171	180	196	rBV	70685	97198	11.72%	1.460%
3	2.575	372	384	400	rBV	140713	231670	27.95%	3.480%
4	3.369	616	631	646	rBV2	11394	26728	3.22%	0.401%
5	4.642	994	1027	1066	rBV2	106829	392984	47.40%	5.903%
6	5.067	1143	1159	1181	rBV	125574	280903	33.88%	4.220%
7	5.729	1344	1365	1385	rBV2	255367	664392	80.14%	9.980%
8	6.253	1512	1528	1554	rBV	205072	397237	47.92%	5.967%
9	6.546	1607	1619	1633	rBV2	36493	68517	8.26%	1.029%
10	6.693	1649	1665	1686	rBV	157649	312070	37.64%	4.688%
11	7.568	1925	1937	1955	rBV2	90715	159263	19.21%	2.392%
12	7.902	2027	2041	2058	rBV	320827	585862	70.67%	8.801%
13	8.182	2115	2128	2143	rBV	57243	95321	11.50%	1.432%
14	8.555	2231	2244	2258	rBV	312578	546592	65.93%	8.211%
15	8.636	2258	2269	2310	rVB	458253	829015	100.00%	12.453%
16	9.420	2495	2513	2540	rBV	303209	526322	63.49%	7.906%
17	10.758	2915	2929	2945	rBV	127547	208818	25.19%	3.137%
18	11.812	3245	3257	3273	rBV	377389	594382	71.70%	8.929%
19	12.195	3360	3376	3398	rBV	331583	536131	64.67%	8.054%




Sum of corrected areas: 6657105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047173.D
Acq On : 16 Feb 2022 20:03
Operator : SY/MD
Sample : N1558-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

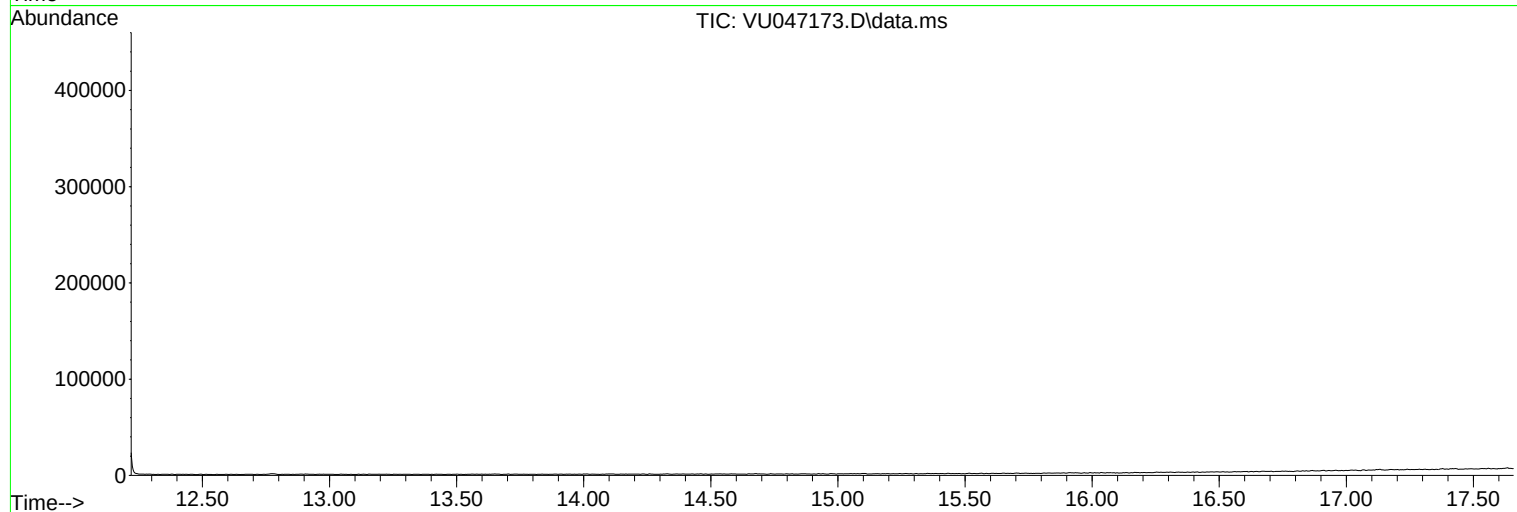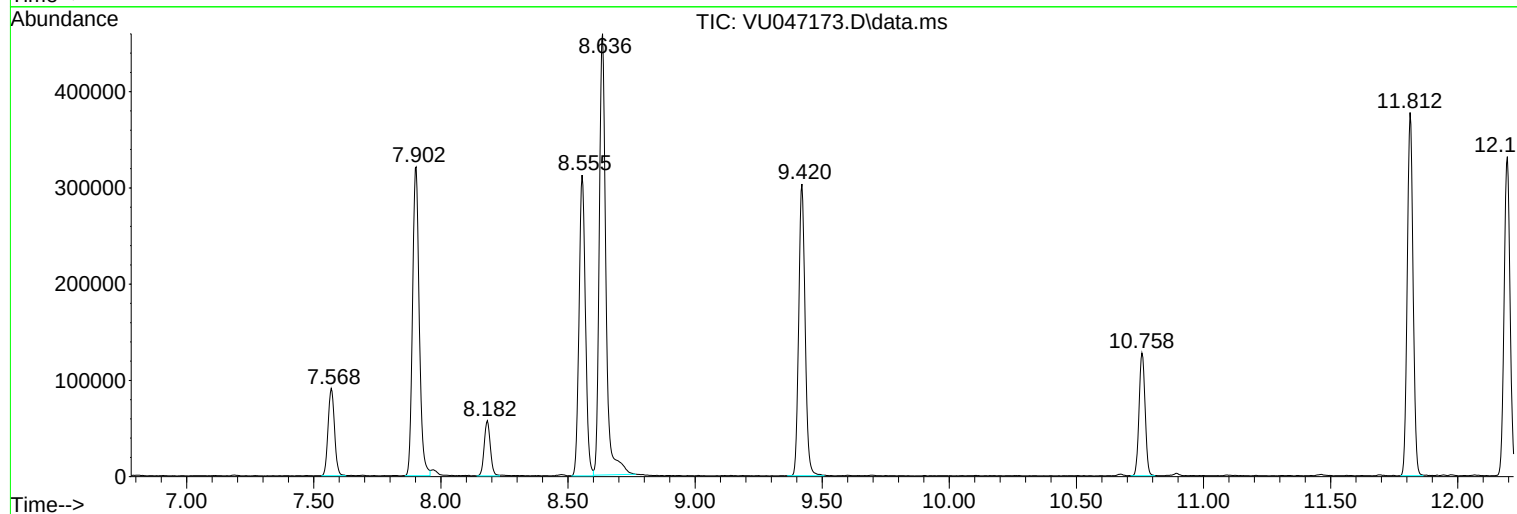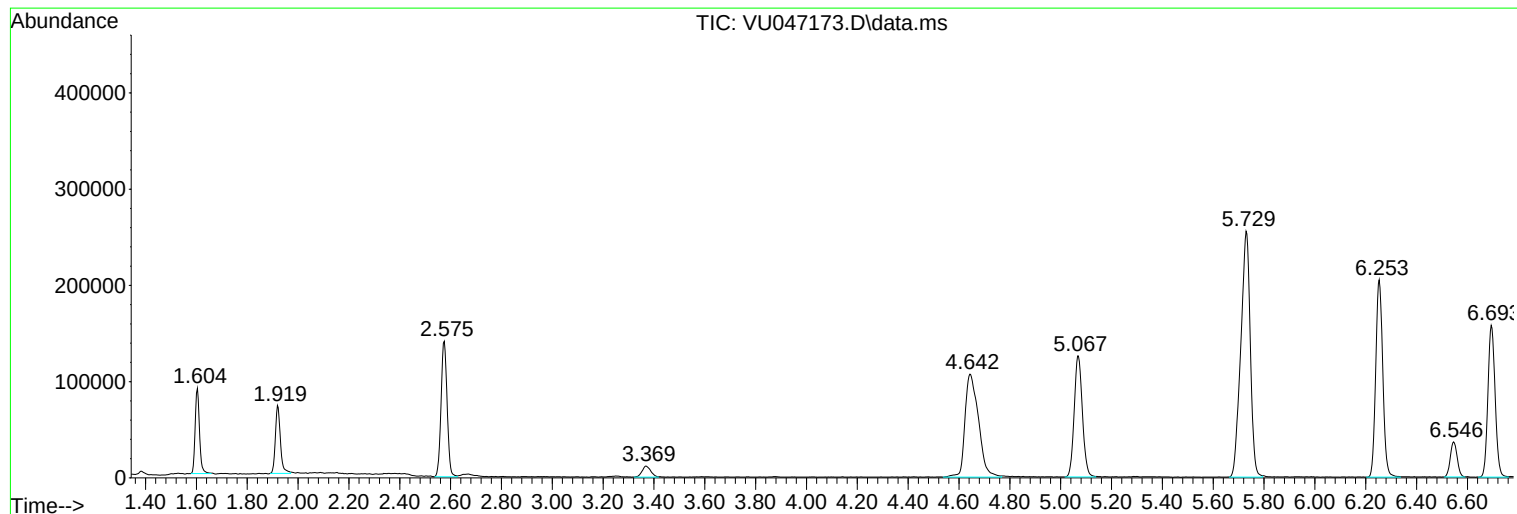

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047173.D
Acq On : 16 Feb 2022 20:03
Operator : SY/MD
Sample : N1558-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047173.D
Acq On : 16 Feb 2022 20:03
Operator : SY/MD
Sample : N1558-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc