

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
 Data File : VU047177.D
 Acq On : 16 Feb 2022 23:39
 Operator : SY/MD
 Sample : N1559-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M85

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	102	rBV	89768	106189	3.68%	1.191%
2	1.919	171	180	191	rBV	69492	93627	3.25%	1.050%
3	2.575	372	384	398	rBV	141781	231157	8.02%	2.592%
4	4.645	1010	1028	1077	rBV	86637	305899	10.61%	3.430%
5	5.070	1140	1160	1184	rBV2	144175	340513	11.81%	3.818%
6	5.729	1342	1365	1393	rBV2	251133	655322	22.72%	7.347%
7	6.253	1514	1528	1554	rBV	196798	376209	13.04%	4.218%
8	6.694	1651	1665	1684	rBV	157122	305265	10.58%	3.422%
9	6.793	1685	1696	1713	rVB2	20203	38588	1.34%	0.433%
10	7.568	1925	1937	1956	rBV	87012	153662	5.33%	1.723%
11	7.903	2025	2041	2051	rBV	314294	567711	19.68%	6.365%
12	7.973	2051	2063	2106	rVB	1564322	2884016	100.00%	32.333%
13	8.182	2115	2128	2141	rVB	55048	92555	3.21%	1.038%
14	8.636	2254	2269	2287	rBV	423513	765904	26.56%	8.587%
15	9.420	2498	2513	2540	rBV	289644	505757	17.54%	5.670%
16	9.693	2588	2598	2613	rBV2	17720	30887	1.07%	0.346%
17	10.079	2708	2718	2745	rBV2	73138	134269	4.66%	1.505%
18	10.758	2918	2929	2947	rBV	124342	200978	6.97%	2.253%
19	11.812	3244	3257	3276	rBV	358486	570223	19.77%	6.393%
20	12.195	3362	3376	3396	rBV	326616	528283	18.32%	5.923%
21	12.889	3581	3592	3603	rBV2	21127	32602	1.13%	0.366%




Sum of corrected areas: 8919616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047177.D
Acq On : 16 Feb 2022 23:39
Operator : SY/MD
Sample : N1559-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

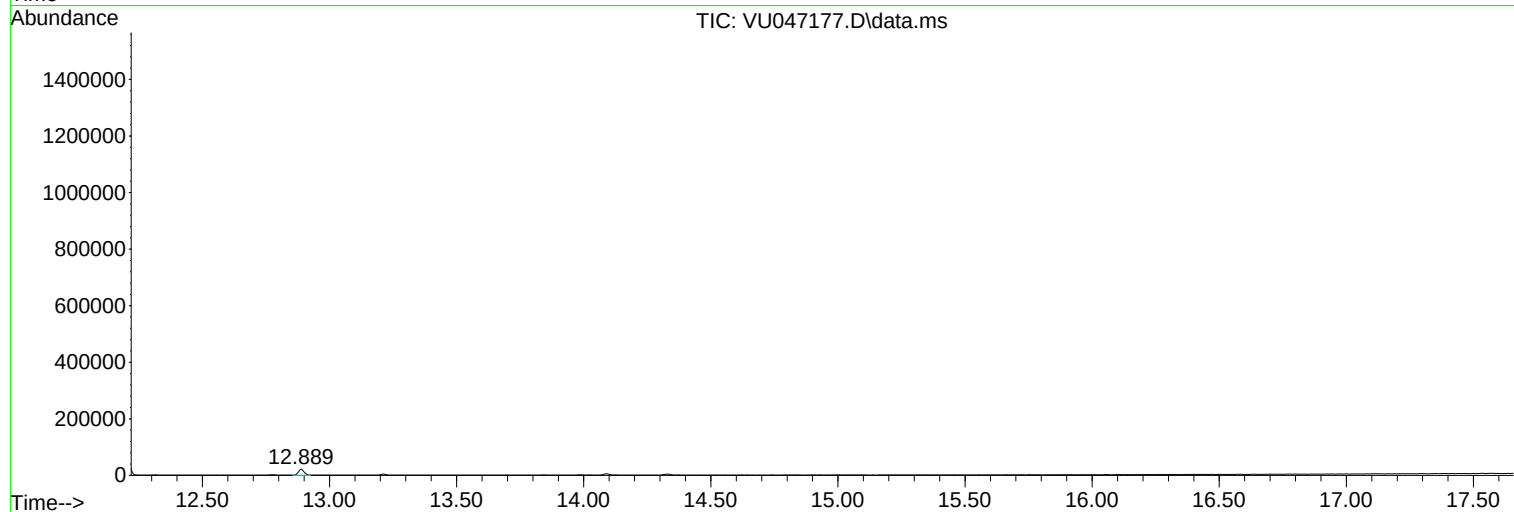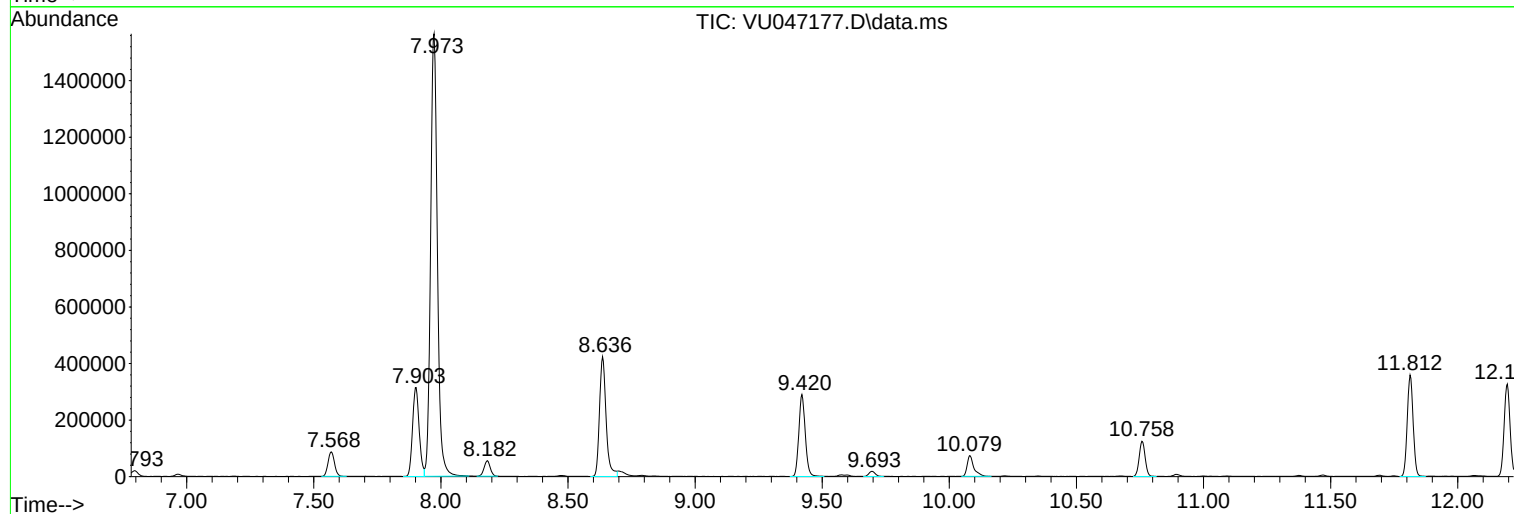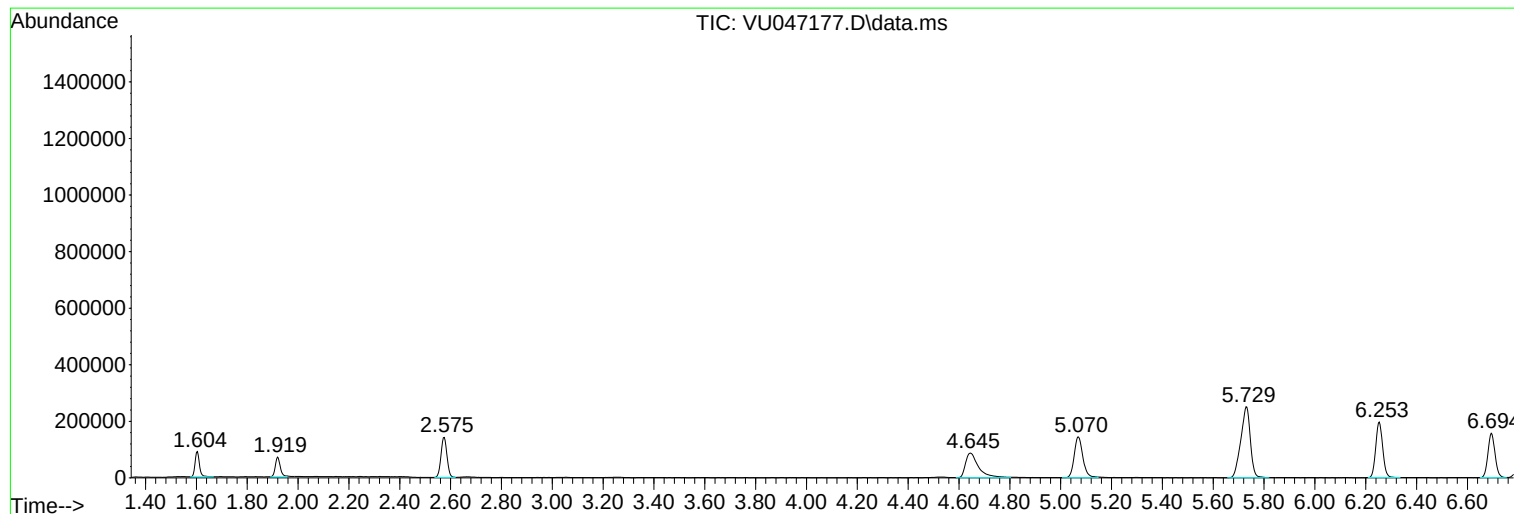

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047177.D
Acq On : 16 Feb 2022 23:39
Operator : SY/MD
Sample : N1559-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047177.D
Acq On : 16 Feb 2022 23:39
Operator : SY/MD
Sample : N1559-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc