

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
 Data File : VU047179.D
 Acq On : 17 Feb 2022 00:28
 Operator : SY/MD
 Sample : N1559-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M54

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	95	rBV	96293	114936	14.16%	1.981%
2	1.919	172	180	201	rBV	67959	93983	11.58%	1.620%
3	2.575	371	384	397	rBV	137359	225577	27.80%	3.887%
4	2.665	401	412	431	rVB	2677	8983	1.11%	0.155%
5	4.642	1012	1027	1069	rBV	93683	305558	37.65%	5.266%
6	5.070	1142	1160	1181	rBV	119818	266096	32.79%	4.586%
7	5.395	1249	1261	1274	rVB5	5999	14068	1.73%	0.242%
8	5.729	1344	1365	1392	rBV2	247513	647836	79.83%	11.164%
9	6.253	1511	1528	1546	rBV	196107	374607	46.16%	6.456%
10	6.694	1651	1665	1684	rBV	155762	299568	36.92%	5.163%
11	7.568	1924	1937	1951	rBV	86369	150739	18.58%	2.598%
12	7.902	2025	2041	2059	rBV	306531	570898	70.35%	9.839%
13	8.182	2116	2128	2143	rBV	54361	89375	11.01%	1.540%
14	8.636	2256	2269	2311	rBV	434578	811507	100.00%	13.985%
15	9.420	2499	2513	2536	rBV	283792	501370	61.78%	8.640%
16	9.693	2589	2598	2612	rBV	11487	18849	2.32%	0.325%
17	10.105	2716	2726	2738	rVB2	6616	10829	1.33%	0.187%
18	10.758	2918	2929	2947	rBV	122846	202598	24.97%	3.491%
19	10.896	2961	2972	2987	rBV	5490	9521	1.17%	0.164%
20	11.812	3243	3257	3274	rBV	358085	564306	69.54%	9.725%
21	12.195	3359	3376	3392	rBV	321247	521450	64.26%	8.986%




Sum of corrected areas: 5802654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047179.D
Acq On : 17 Feb 2022 00:28
Operator : SY/MD
Sample : N1559-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

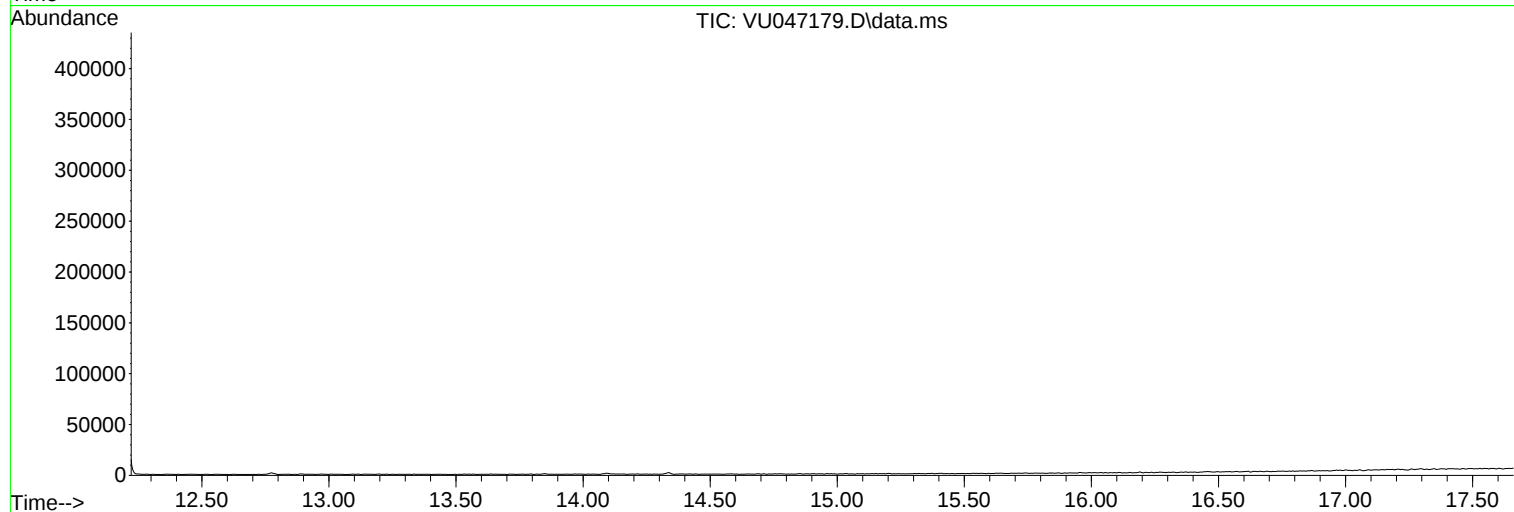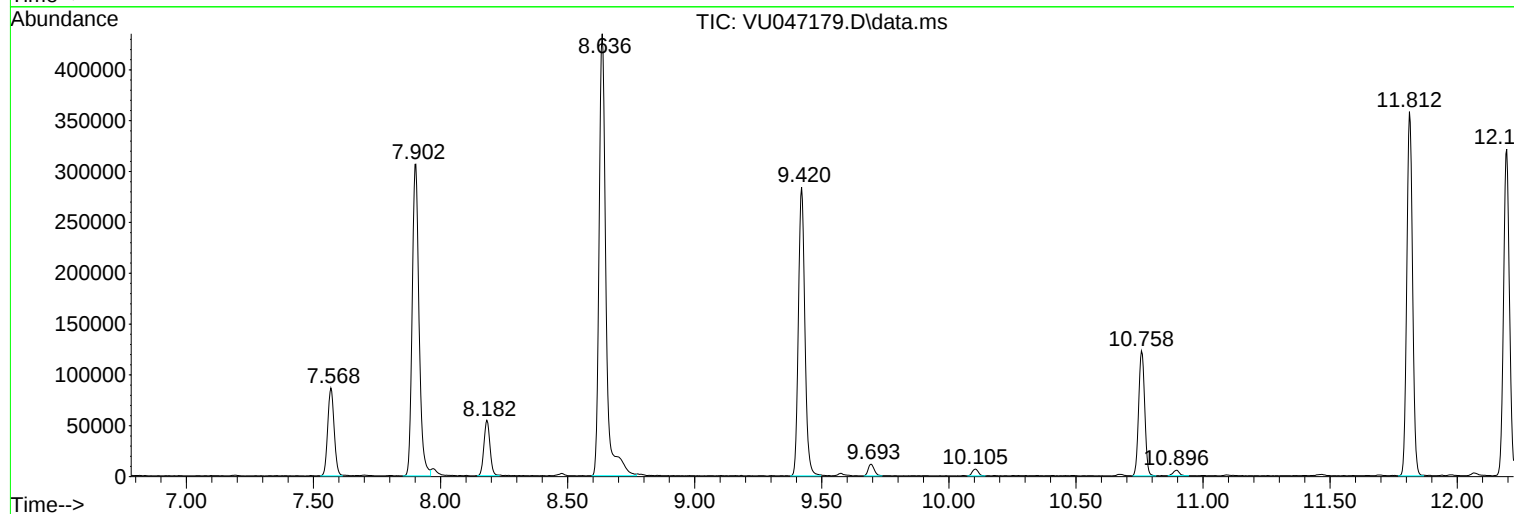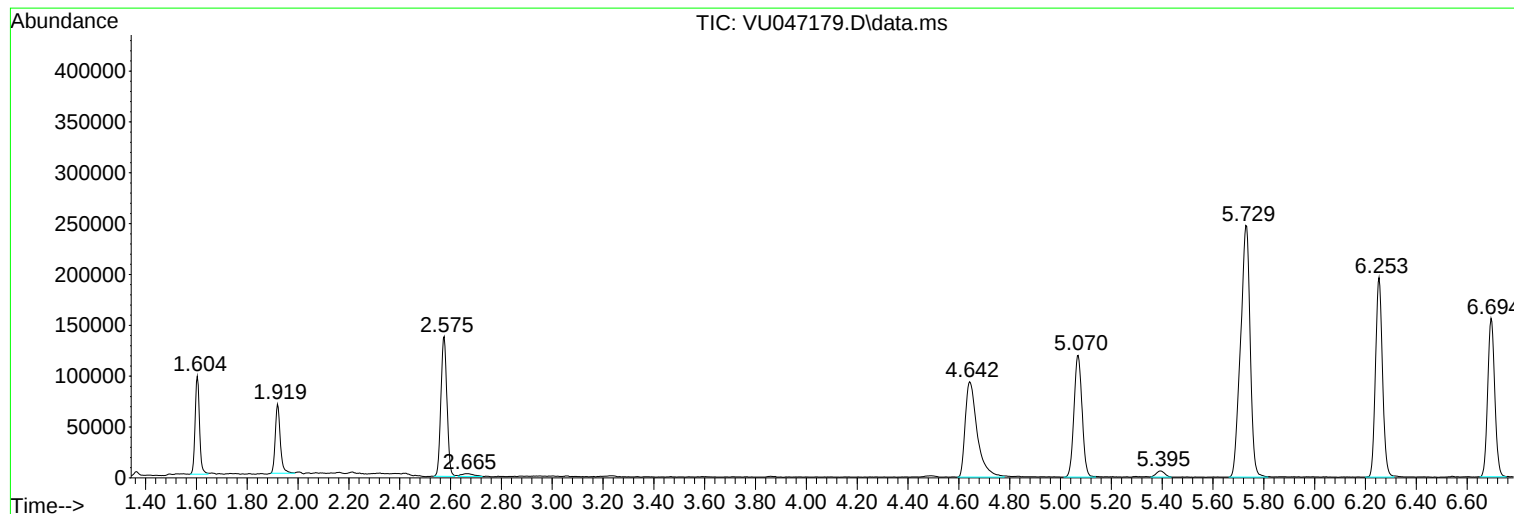

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047179.D
Acq On : 17 Feb 2022 00:28
Operator : SY/MD
Sample : N1559-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047179.D
Acq On : 17 Feb 2022 00:28
Operator : SY/MD
Sample : N1559-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
