

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
 Data File : VU047189.D
 Acq On : 17 Feb 2022 04:28
 Operator : SY/MD
 Sample : N1558-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M94

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rBV	81426	94390	3.31%	1.108%
2	1.919	172	180	198	rBV	65643	89668	3.15%	1.053%
3	2.575	371	384	399	rBV	129988	213759	7.50%	2.509%
4	4.645	1013	1028	1069	rBV	81718	293776	10.30%	3.449%
5	5.070	1141	1160	1193	rBV2	136111	326748	11.46%	3.836%
6	5.729	1344	1365	1393	rBV2	237936	616375	21.62%	7.236%
7	6.253	1514	1528	1552	rBV	183040	349137	12.25%	4.099%
8	6.694	1651	1665	1685	rBV	148559	288242	10.11%	3.384%
9	6.793	1685	1696	1713	rVB2	18474	34697	1.22%	0.407%
10	7.568	1924	1937	1953	rBV	81132	142708	5.01%	1.675%
11	7.903	2027	2041	2051	rBV	289147	529322	18.57%	6.214%
12	7.973	2051	2063	2099	rVB	1523098	2850931	100.00%	33.468%
13	8.182	2117	2128	2147	rVB	51244	87248	3.06%	1.024%
14	8.636	2255	2269	2288	rBV	413466	754623	26.47%	8.859%
15	9.420	2500	2513	2540	rBV	267139	470067	16.49%	5.518%
16	9.697	2589	2599	2611	rVB	17352	28642	1.00%	0.336%
17	10.079	2708	2718	2744	rBV2	67453	126190	4.43%	1.481%
18	10.758	2915	2929	2947	rVB	119653	195551	6.86%	2.296%
19	11.812	3245	3257	3274	rBV	334414	528590	18.54%	6.205%
20	12.195	3362	3376	3392	rBV	307133	497672	17.46%	5.842%




Sum of corrected areas: 8518336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047189.D
Acq On : 17 Feb 2022 04:28
Operator : SY/MD
Sample : N1558-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

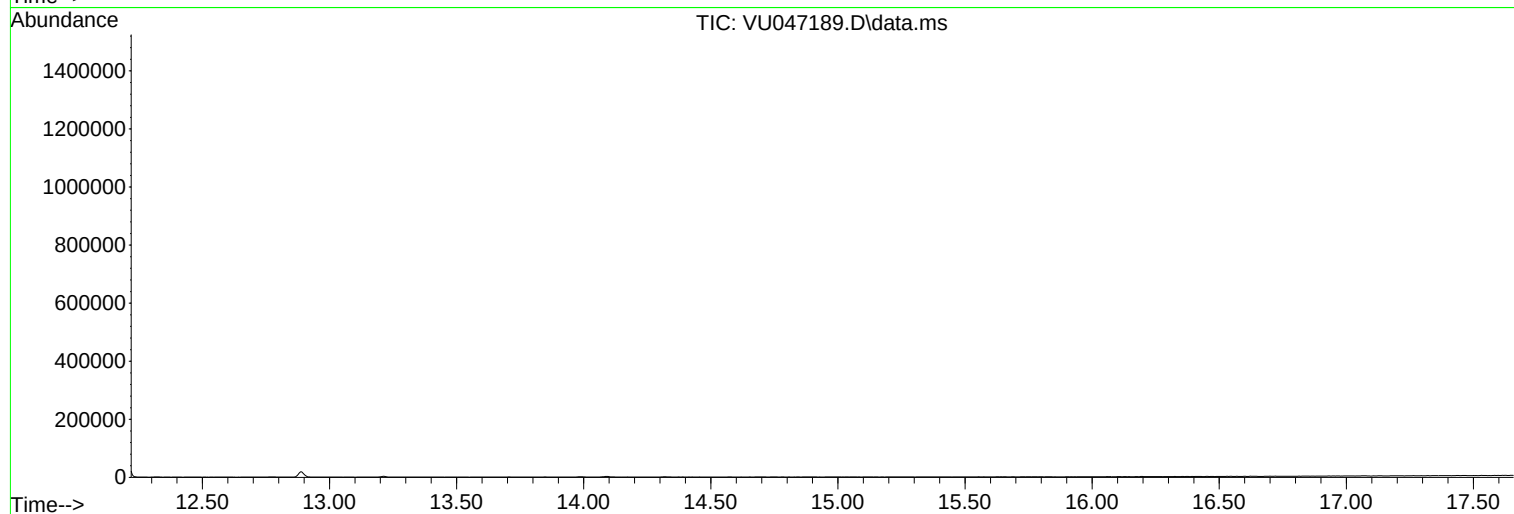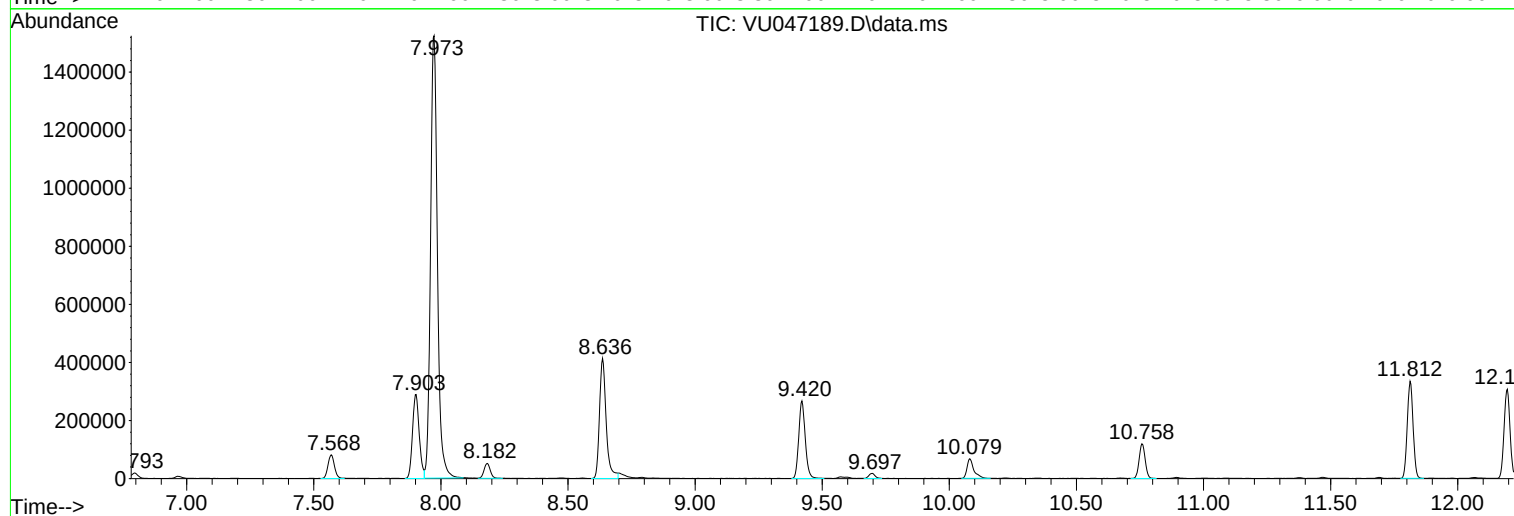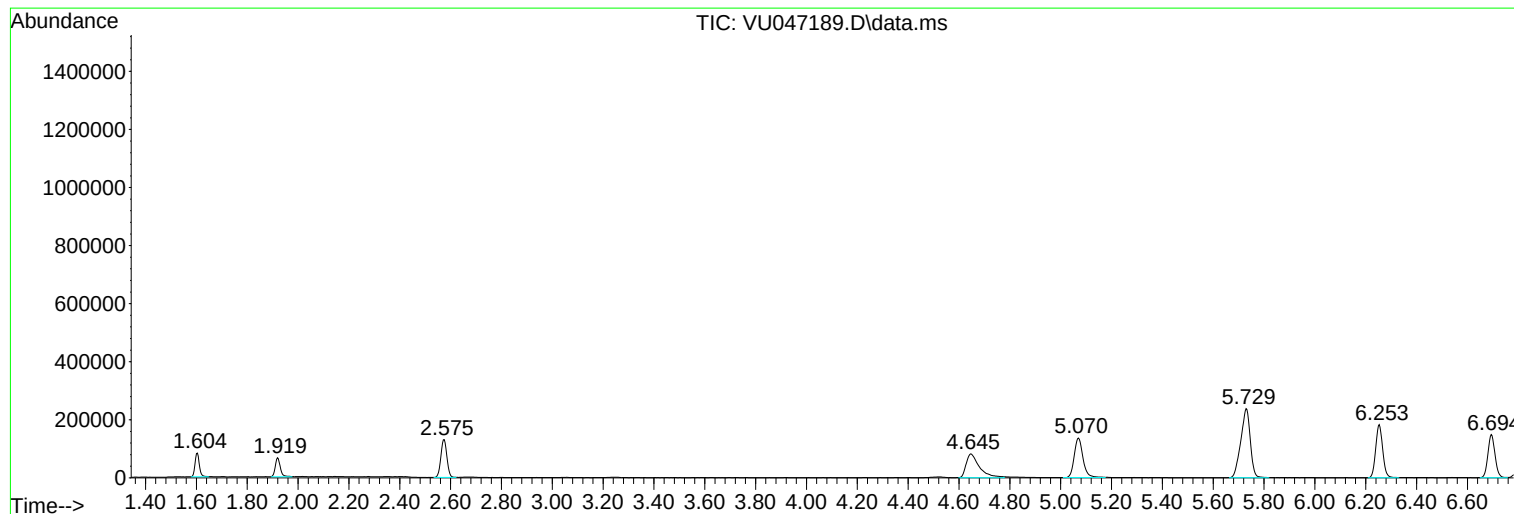

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047189.D
Acq On : 17 Feb 2022 04:28
Operator : SY/MD
Sample : N1558-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
Data File : VU047189.D
Acq On : 17 Feb 2022 04:28
Operator : SY/MD
Sample : N1558-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
