


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021622\
 Data File : VU047152.D
 Acq On : 16 Feb 2022 09:04
 Operator : SY/MD
 Sample : BFB056
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB056

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Mar 01 00:43:41 2022

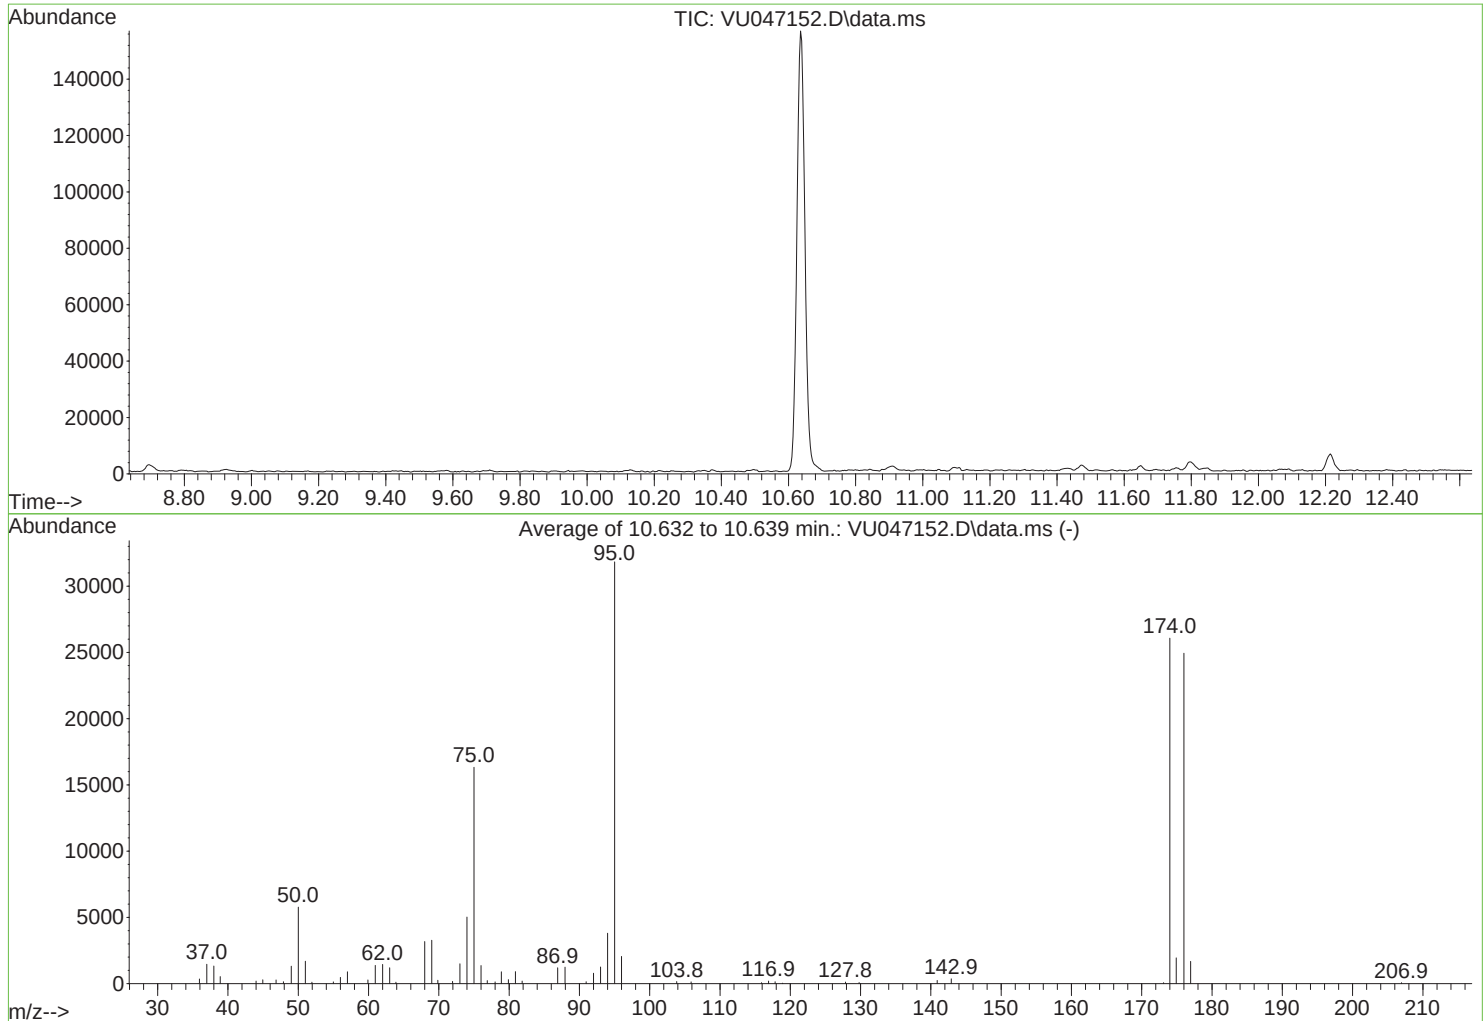

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5777	PASS
75	95	30	80	51.3	16330	PASS
95	95	100	100	100.0	31832	PASS
96	95	5	9	6.4	2050	PASS
173	174	0.00	2	0.3	75	PASS
174	95	50	120	81.9	26075	PASS
175	174	5	9	7.5	1949	PASS
176	174	95	101	95.6	24933	PASS
177	176	5	9	6.8	1684	PASS

m/z	Abundance
35.90	103.0
40.00	120.0
44.00	395.0
207.00	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
36.00	469.0
37.00	1492.0
38.00	1305.0
38.90	584.0
40.00	115.0
44.00	627.0
45.00	283.0
46.90	244.0
47.90	148.0
49.00	1268.0
50.00	5662.0
51.00	1581.0
51.90	107.0
55.00	131.0
56.00	447.0
57.00	891.0
59.90	288.0
61.00	1375.0
62.00	1468.0
63.00	1156.0
63.90	105.0
68.00	3015.0
69.00	3202.0
69.90	277.0
72.00	169.0
73.00	1297.0
74.00	4848.0
75.00	15892.0
76.00	1315.0
76.90	234.0
78.00	165.0
78.90	884.0
79.90	291.0
80.90	899.0
81.90	194.0
86.90	1212.0
87.90	1292.0
90.90	162.0
92.00	695.0
93.00	1281.0
94.00	3598.0
95.00	31080.0
96.00	1984.0
103.90	129.0
105.80	129.0
115.90	126.0
116.90	196.0
117.80	147.0
118.90	130.0
127.90	124.0
140.90	233.0
142.90	337.0
174.00	24600.0
174.90	1886.0
176.00	23776.0
177.00	1700.0
206.90	351.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
36.00	441.0
37.00	1416.0
38.00	1309.0
38.90	462.0
39.90	128.0
44.00	556.0
44.90	292.0
46.90	321.0
47.90	147.0
49.00	1347.0
50.00	5740.0
51.00	1753.0
52.00	111.0
55.00	136.0
56.00	471.0
57.00	857.0
59.90	272.0
60.90	1350.0
62.00	1366.0
63.00	1185.0
63.90	105.0
68.00	3252.0
69.00	3225.0
69.90	224.0
71.90	164.0
73.00	1631.0
74.00	5060.0
75.00	16257.0
76.00	1383.0
76.90	214.0
78.00	106.0
78.90	884.0
79.90	297.0
80.90	901.0
81.80	197.0
86.90	1160.0
88.00	1193.0
91.00	118.0
92.00	839.0
93.00	1193.0
94.00	3864.0
95.00	31712.0
96.00	2073.0
103.80	165.0
106.00	136.0
116.90	196.0
117.90	130.0
127.80	121.0
129.80	141.0
140.90	241.0
142.90	362.0
173.10	224.0
174.00	26784.0
174.90	1911.0
176.00	25432.0
176.90	1641.0
207.00	381.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
36.00	447.0
37.00	1483.0
38.00	1384.0
38.90	542.0
39.90	109.0
44.00	587.0
44.90	301.0
46.80	290.0
47.90	158.0
49.00	1340.0
50.00	5929.0
51.00	1756.0
52.00	112.0
55.00	126.0
56.00	494.0
57.00	929.0
59.90	290.0
61.00	1407.0
62.00	1506.0
63.00	1242.0
63.90	106.0
68.00	3278.0
69.00	3410.0
69.80	253.0
72.00	168.0
73.00	1562.0
74.00	5150.0
75.00	16840.0
76.00	1413.0
76.90	235.0
78.00	138.0
78.90	911.0
79.90	310.0
80.90	936.0
81.80	203.0
86.90	1231.0
88.00	1262.0
90.90	161.0
92.00	819.0
93.00	1315.0
94.00	3943.0
95.00	32704.0
96.00	2092.0
103.90	161.0
105.90	132.0
115.90	101.0
116.90	200.0
117.90	147.0
127.90	119.0
129.80	125.0
140.90	234.0
142.90	391.0
174.00	26840.0
174.90	2049.0
176.00	25592.0
176.90	1712.0
207.00	366.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056