


Acrolein

Response Ratio

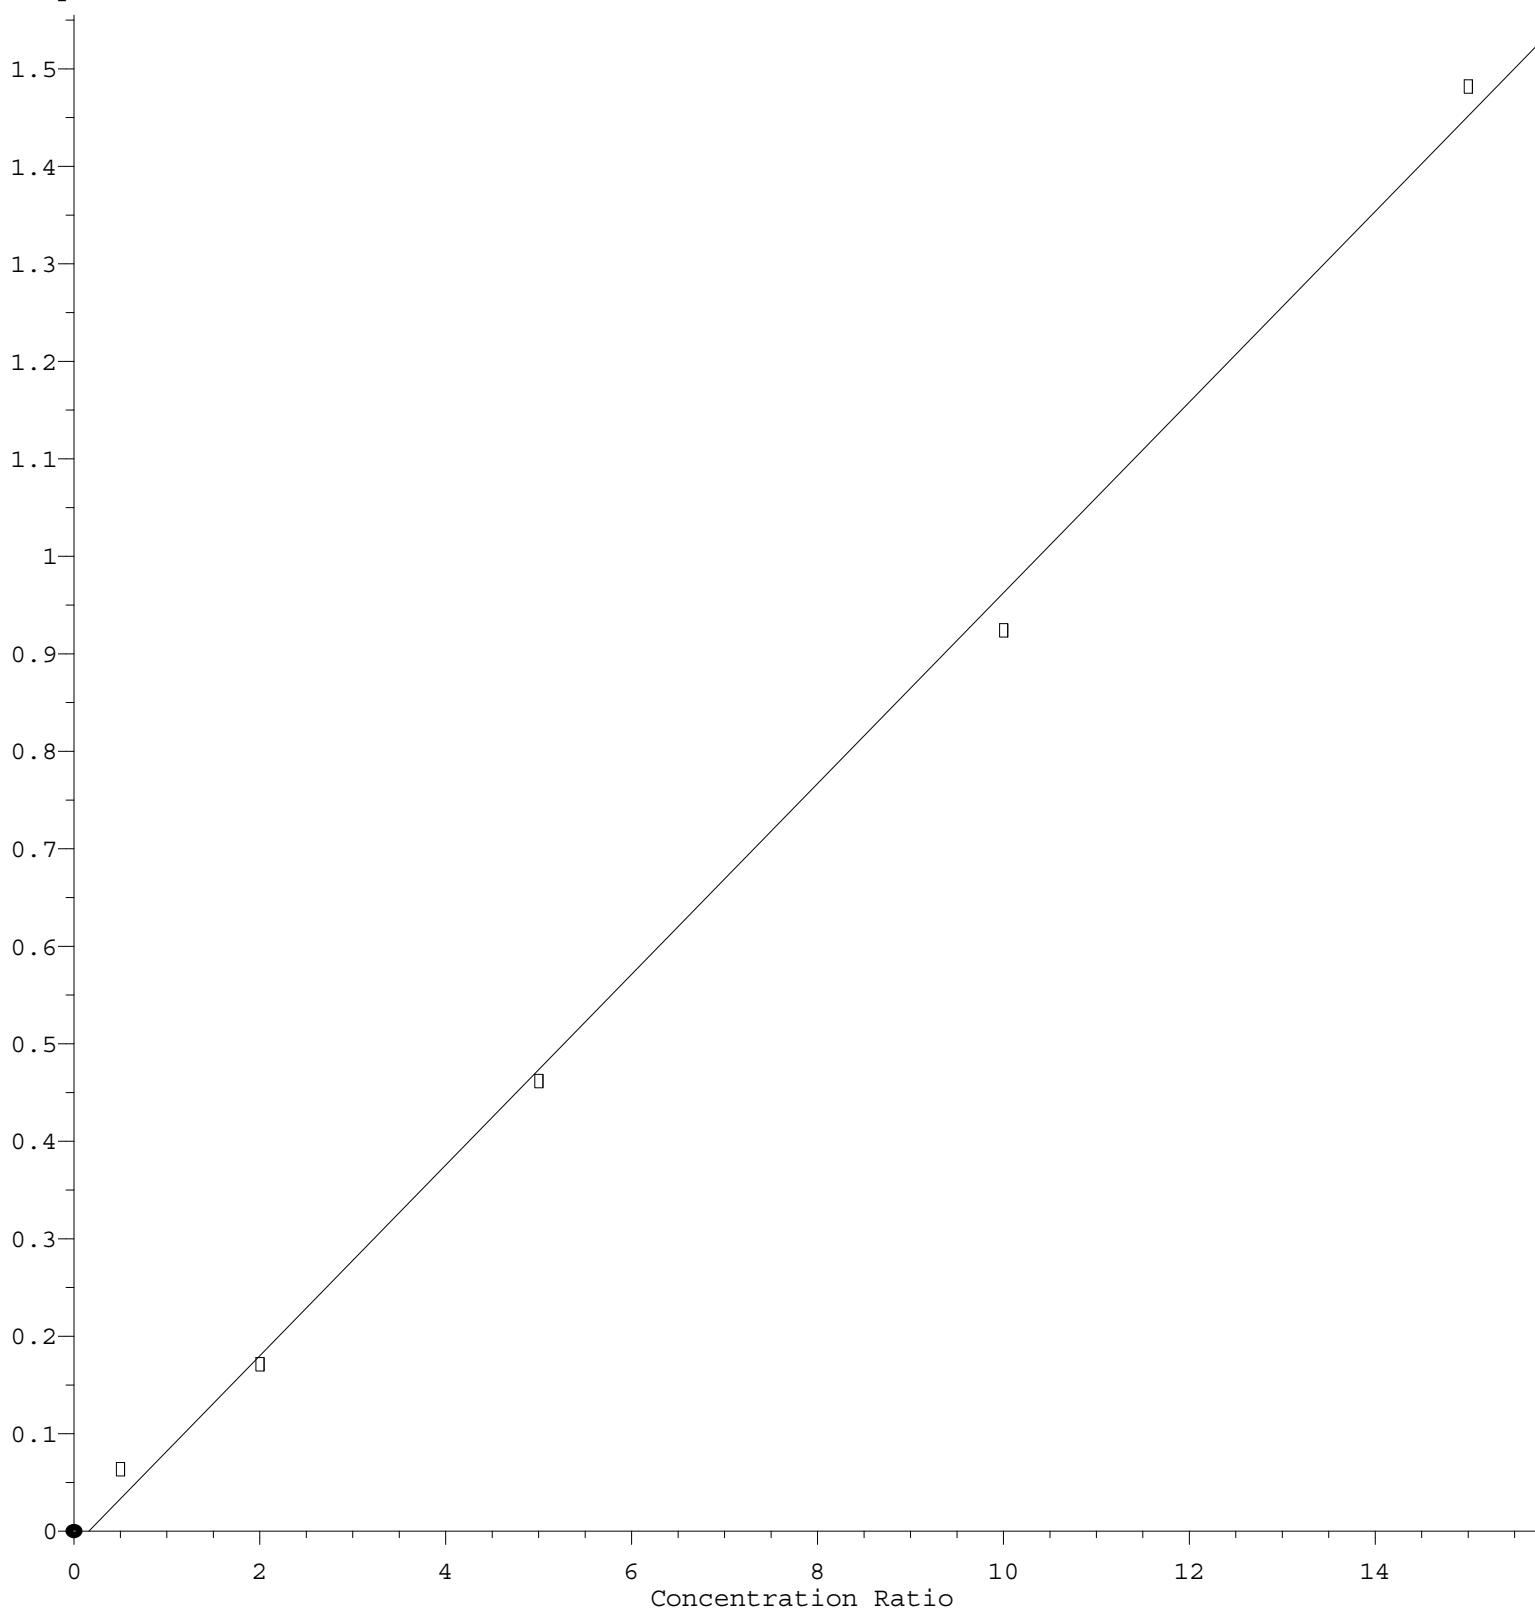

$$\text{Response} = 9.780\text{e-}002 * \text{Amt} - 1.529\text{e-}002$$


Coef of Det (r^2) = 0.997428 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\82U021721W.M

Calibration Table Last Updated: Fri Feb 19 02:55:52 2021

2-Chloroethyl Vinyl ether

Response Ratio

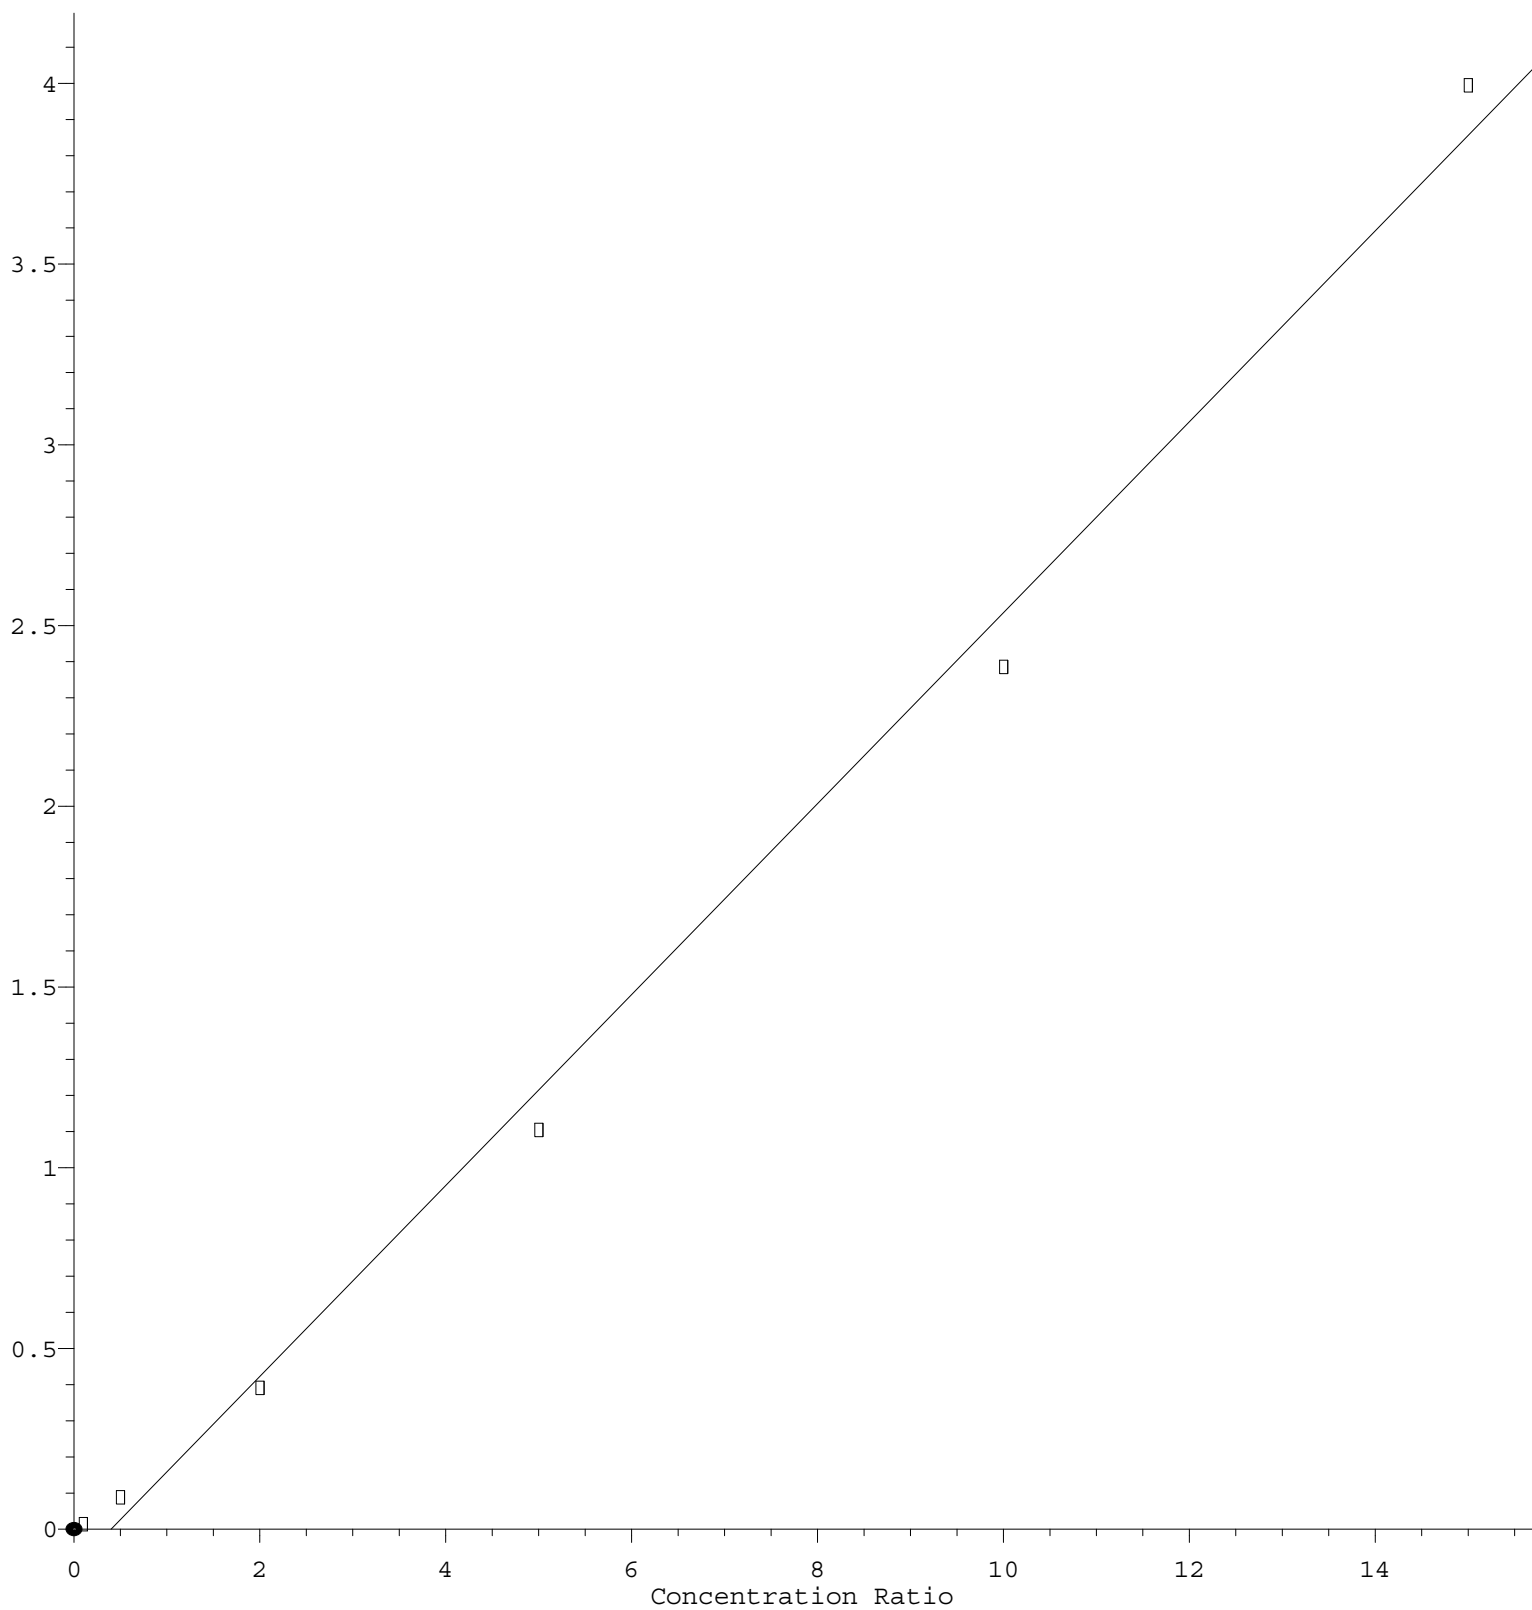

$$\text{Response} = 2.641\text{e-}001 * \text{Amt} - 1.055\text{e-}001$$


Coef of Det (r^2) = 0.994576 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\82U021721W.M

Calibration Table Last Updated: Fri Feb 19 02:55:52 2021

1,2,4-Trichlorobenzene

Response Ratio

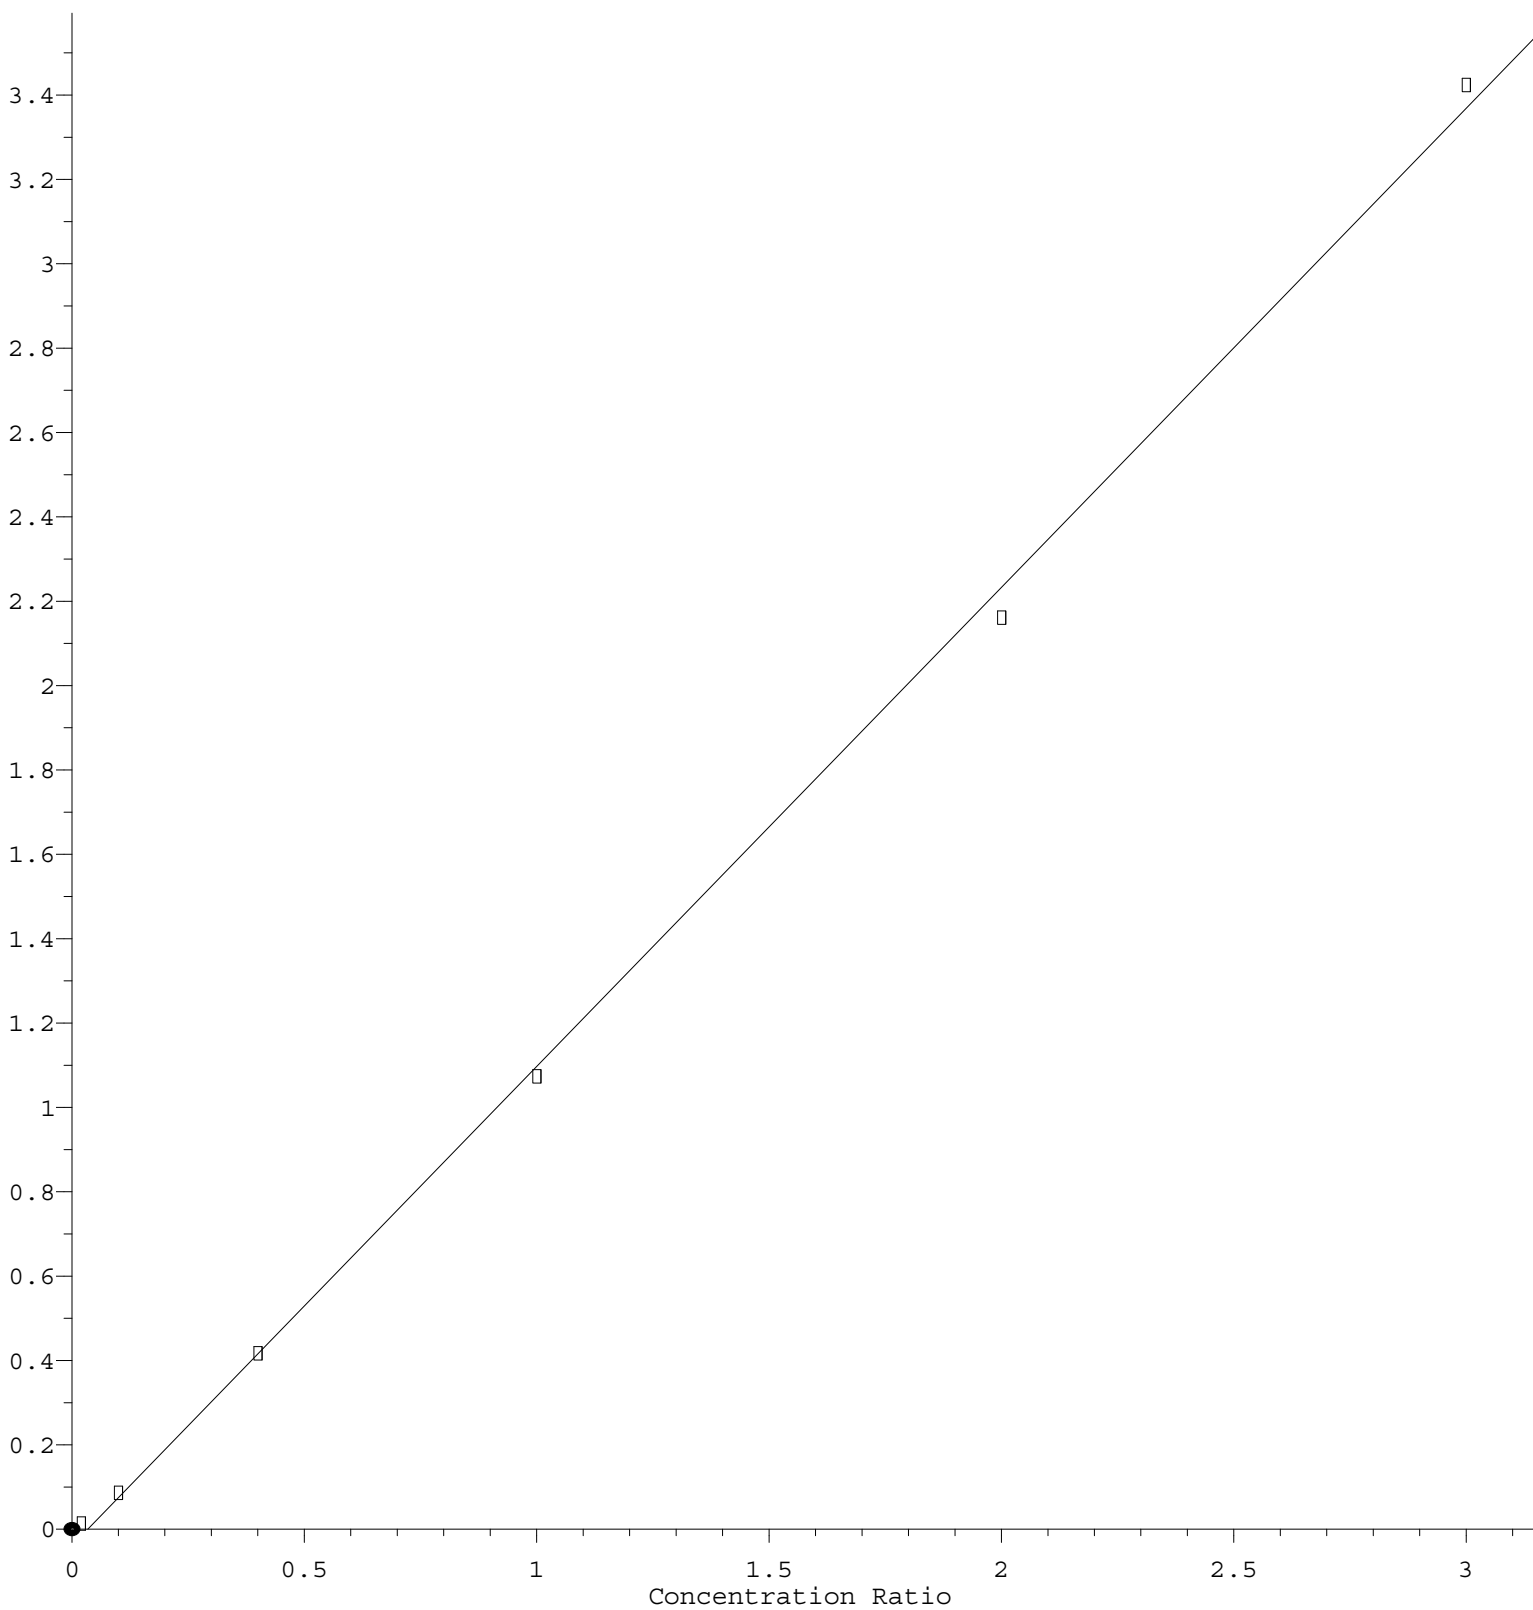

$$\text{Response} = 1.136 \times 10^0 \times \text{Amt} - 3.831 \times 10^{-02}$$


Coef of Det (r^2) = 0.998936 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\82U021721W.M

Calibration Table Last Updated: Fri Feb 19 02:55:52 2021

Naphthalene

Response Ratio

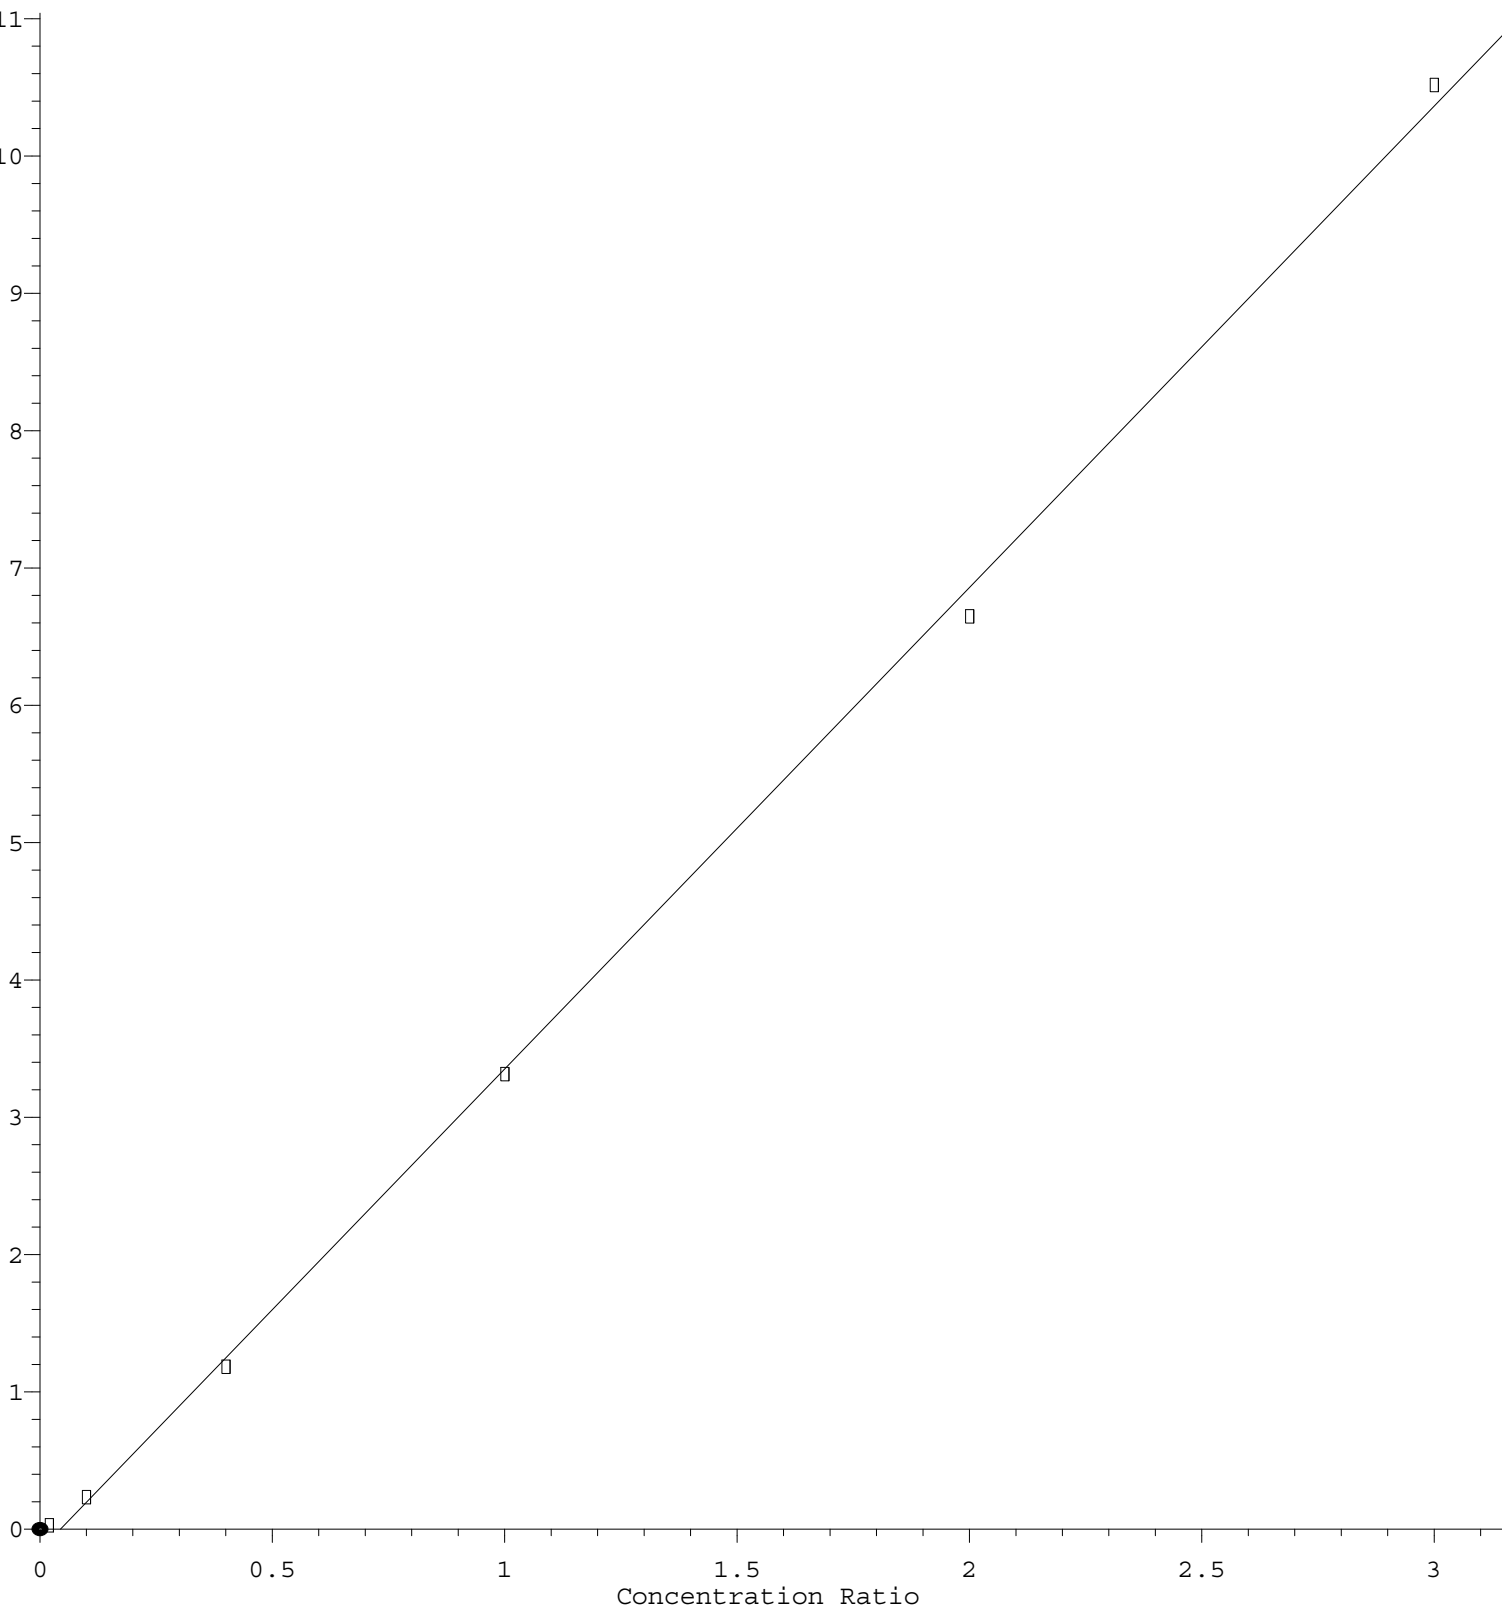

$$\text{Response} = 3.505\text{e}+000 * \text{Amt} - 1.551\text{e}-001$$


Coef of Det (r^2) = 0.998996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\82U021721W.M

Calibration Table Last Updated: Fri Feb 19 02:55:52 2021

1,2,3-Trichlorobenzene

Response Ratio

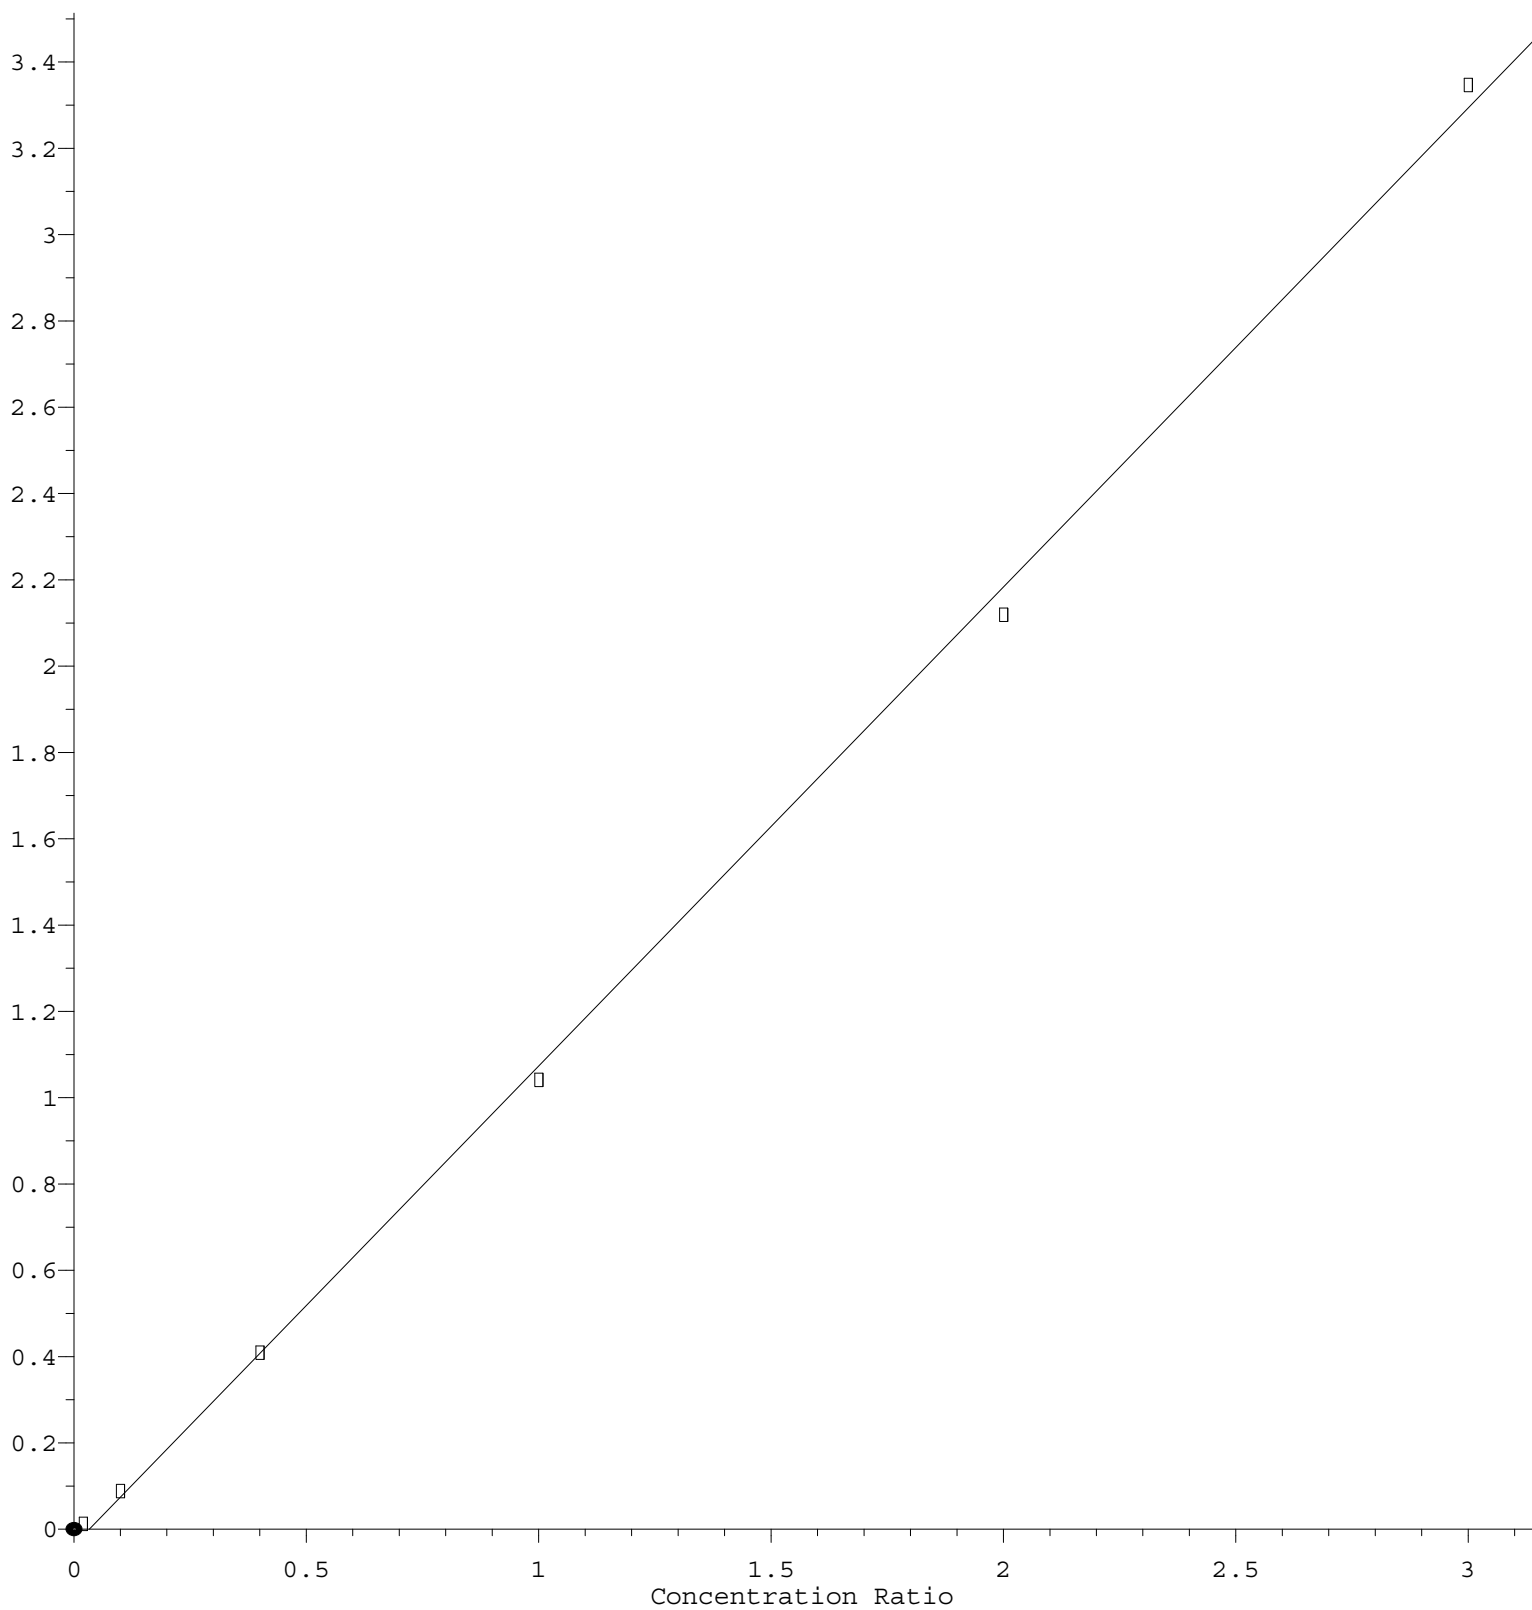

$$\text{Response} = 1.110\text{e}+000 * \text{Amt} - 3.719\text{e}-002$$

Coef of Det (r^2) = 0.998980 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\82U021721W.M

Calibration Table Last Updated: Fri Feb 19 02:55:52 2021