


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021721\
 Data File : VU042320.D
 Acq On : 17 Feb 2021 08:52
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
 Title : SW846 8260
 Last Update : Fri Feb 19 02:55:52 2021

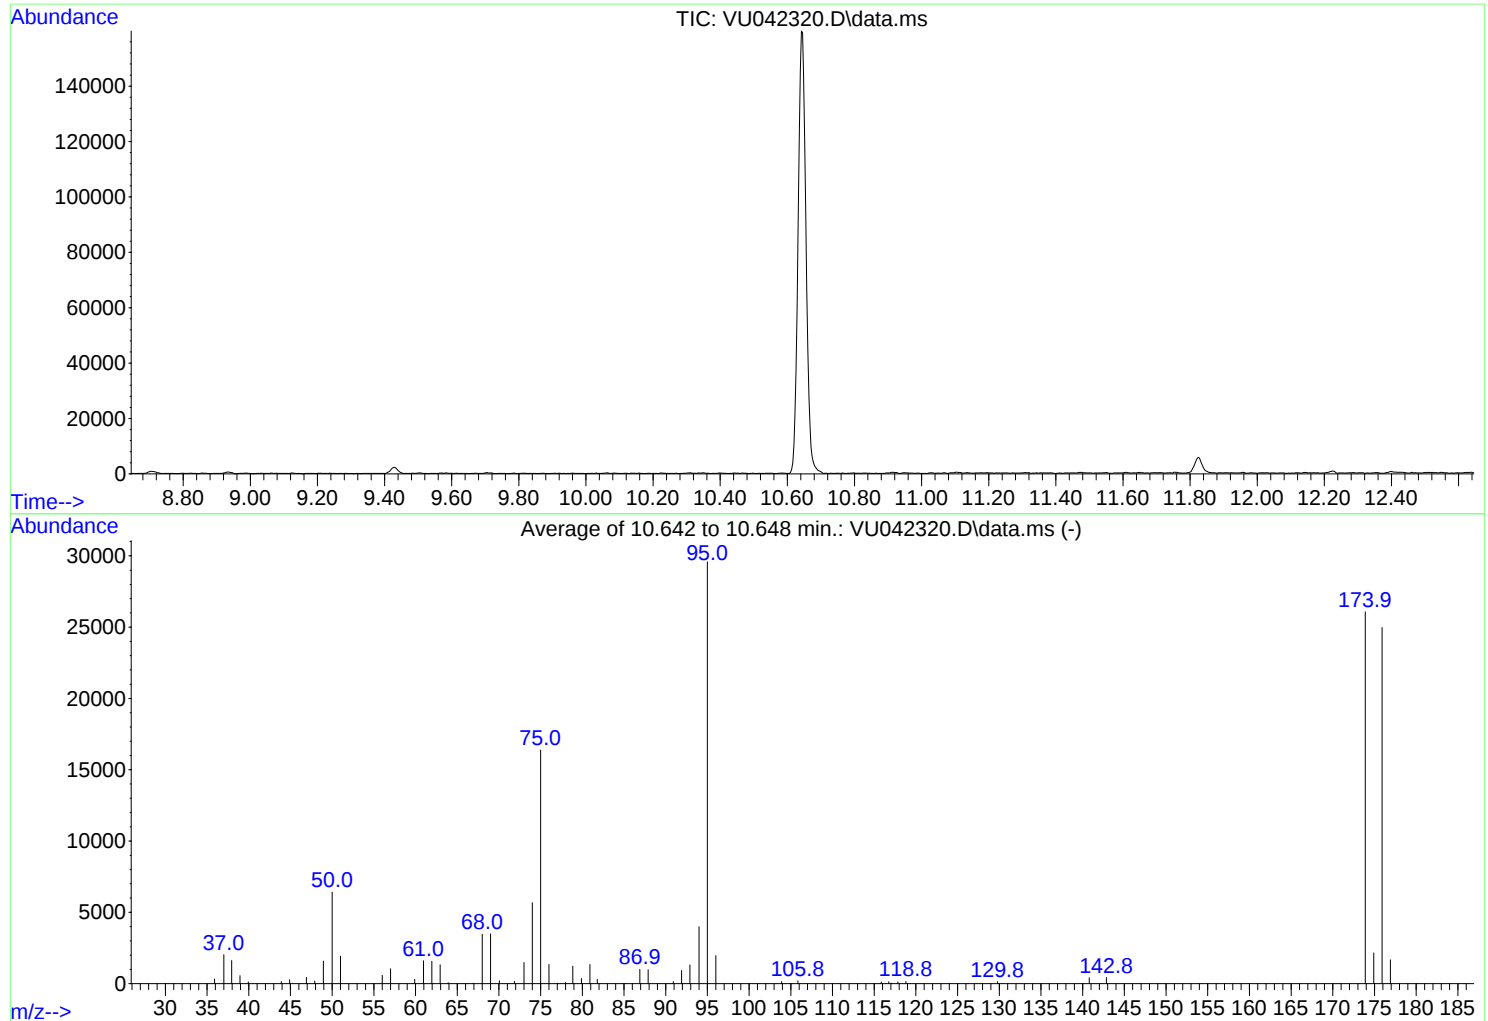

AutoFind: Scans 2893, 2894, 2895; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	6420	PASS
75	95	30	60	55.4	16382	PASS
95	95	100	100	100.0	29581	PASS
96	95	5	9	6.6	1961	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.1	26075	PASS
175	174	5	9	8.3	2152	PASS
176	174	95	101	95.8	24976	PASS
177	176	5	9	6.7	1676	PASS