

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047196.D
 Acq On : 17 Feb 2022 10:48
 Operator : SY/MD
 Sample : VU0217WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	102	rBV	188279	223023	14.09%	1.777%
2	1.919	171	180	207	rVB	164750	233787	14.76%	1.863%
3	2.572	371	383	406	rBV	309081	519059	32.78%	4.135%
4	2.842	461	467	469	rBV	260	223	0.01%	0.002%
5	2.864	471	474	478	rBV2	246	253	0.02%	0.002%
6	2.906	482	487	490	rBV2	274	252	0.02%	0.002%
7	2.941	494	498	499	rBV2	369	272	0.02%	0.002%
8	3.054	528	533	540	rVB4	979	1061	0.07%	0.008%
9	3.128	553	556	562	rVB2	310	320	0.02%	0.003%
10	3.350	622	625	630	rBV	400	407	0.03%	0.003%
11	3.601	700	703	706	rBV	297	249	0.02%	0.002%
12	3.691	726	731	733	rBV2	206	210	0.01%	0.002%
13	3.745	745	748	753	rBV2	300	313	0.02%	0.002%
14	3.874	783	788	792	rBV2	163	208	0.01%	0.002%
15	3.948	805	811	817	rBV2	243	339	0.02%	0.003%
16	3.983	817	822	825	rBV3	208	221	0.01%	0.002%
17	4.279	910	914	919	rBV3	218	233	0.01%	0.002%
18	4.356	932	938	940	rBV2	190	198	0.01%	0.002%
19	4.498	975	982	986	rBV2	310	415	0.03%	0.003%
20	4.546	993	997	1002	rVB3	265	253	0.02%	0.002%
21	4.629	1008	1023	1056	rBV	182954	456362	28.82%	3.636%
22	4.867	1094	1097	1102	rBV4	385	320	0.02%	0.003%
23	5.067	1142	1159	1180	rBV	284012	616551	38.94%	4.912%
24	5.202	1198	1201	1204	rVB2	501	284	0.02%	0.002%
25	5.221	1204	1207	1211	rBV2	514	355	0.02%	0.003%
26	5.289	1225	1228	1230	rBV3	633	507	0.03%	0.004%
27	5.440	1269	1275	1280	rBV3	291	478	0.03%	0.004%
28	5.507	1294	1296	1303	rVB3	286	271	0.02%	0.002%
29	5.536	1303	1305	1310	rBV2	227	191	0.01%	0.002%
30	5.594	1319	1323	1328	rBV2	165	183	0.01%	0.001%
31	5.729	1342	1365	1396	rBV2	585287	1583391	100.00%	12.615%
32	6.253	1513	1528	1558	rVV	415584	796738	50.32%	6.348%
33	6.536	1606	1616	1624	rBV2	2905	6448	0.41%	0.051%
34	6.694	1650	1665	1687	rBV	372995	720351	45.49%	5.739%
35	6.806	1694	1700	1710	rBV5	1285	2234	0.14%	0.018%
36	6.970	1749	1751	1756	rVB2	256	221	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047196.D
 Acq On : 17 Feb 2022 10:48
 Operator : SY/MD
 Sample : VU0217WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	7.028	1763	1769	1771	rBV2	624	561	0.04%	0.004%
38	7.044	1771	1774	1784	rVB4	601	943	0.06%	0.008%
39	7.186	1810	1818	1830	rBV4	2322	4062	0.26%	0.032%
40	7.288	1848	1850	1857	rVB2	222	264	0.02%	0.002%
41	7.568	1924	1937	1960	rBV	231804	401717	25.37%	3.201%
42	7.649	1960	1962	1966	rVV	723	658	0.04%	0.005%
43	7.687	1970	1974	1986	rVB7	1922	3121	0.20%	0.025%
44	7.899	2027	2040	2059	rBV	706957	1330908	84.05%	10.604%
45	8.182	2116	2128	2148	rBV	162022	270927	17.11%	2.159%
46	8.308	2163	2167	2169	rBV2	347	325	0.02%	0.003%
47	8.343	2176	2178	2182	rVB3	479	278	0.02%	0.002%
48	8.366	2182	2185	2187	rBV2	416	263	0.02%	0.002%
49	8.427	2200	2204	2210	rBV3	393	337	0.02%	0.003%
50	8.555	2240	2244	2248	rBV2	478	346	0.02%	0.003%
51	8.632	2256	2268	2284	rBV	575480	977642	61.74%	7.789%
52	8.835	2329	2331	2337	rVB4	359	289	0.02%	0.002%
53	9.166	2431	2434	2442	rVB2	300	360	0.02%	0.003%
54	9.353	2487	2492	2496	rBV3	142	193	0.01%	0.002%
55	9.420	2499	2513	2546	rVV	583048	1037335	65.51%	8.265%
56	9.578	2556	2562	2567	rBV2	370	569	0.04%	0.005%
57	9.600	2567	2569	2574	rVV3	309	232	0.01%	0.002%
58	9.694	2593	2598	2607	rVB3	1077	1639	0.10%	0.013%
59	10.099	2720	2724	2727	rBV4	387	382	0.02%	0.003%
60	10.157	2737	2742	2744	rBV2	236	225	0.01%	0.002%
61	10.211	2754	2759	2761	rBV	307	193	0.01%	0.002%
62	10.414	2817	2822	2827	rBV2	324	371	0.02%	0.003%
63	10.671	2896	2902	2911	rBV2	2895	4141	0.26%	0.033%
64	10.758	2916	2929	2948	rBV	545798	887167	56.03%	7.068%
65	10.835	2950	2953	2955	rVB3	501	273	0.02%	0.002%
66	10.874	2960	2965	2969	rBV5	679	786	0.05%	0.006%
67	10.993	2999	3002	3005	rBV3	277	223	0.01%	0.002%
68	11.012	3005	3008	3013	rVB3	288	308	0.02%	0.002%
69	11.057	3017	3022	3024	rBV2	334	283	0.02%	0.002%
70	11.092	3028	3033	3035	rBV2	468	527	0.03%	0.004%
71	11.208	3066	3069	3072	rBV	309	182	0.01%	0.001%
72	11.301	3093	3098	3102	rBV3	347	396	0.03%	0.003%
73	11.378	3118	3122	3129	rVB3	441	504	0.03%	0.004%
74	11.411	3129	3132	3133	rBV2	327	186	0.01%	0.001%
75	11.465	3139	3149	3160	rVB6	2851	5958	0.38%	0.047%
76	11.697	3213	3221	3227	rVB4	1361	1949	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047196.D
 Acq On : 17 Feb 2022 10:48
 Operator : SY/MD
 Sample : VU0217WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.748	3232	3237	3239	rBV2	693	621	0.04%	0.005%
78	11.812	3245	3257	3286	rBV	724608	1137962	71.87%	9.066%
79	11.919	3286	3290	3291	rBV3	381	287	0.02%	0.002%
80	11.944	3291	3298	3302	rVV4	1022	1657	0.10%	0.013%
81	11.973	3303	3307	3313	rVB2	2087	2276	0.14%	0.018%
82	12.118	3350	3352	3357	rVB4	334	200	0.01%	0.002%
83	12.195	3362	3376	3397	rVV	793596	1291807	81.58%	10.292%
84	12.433	3444	3450	3455	rBV	330	341	0.02%	0.003%
85	12.687	3522	3529	3531	rBV2	334	409	0.03%	0.003%
86	12.726	3537	3541	3543	rBV2	274	193	0.01%	0.002%
87	13.144	3667	3671	3676	rBV4	627	532	0.03%	0.004%
88	13.227	3691	3697	3699	rBV3	804	859	0.05%	0.007%
89	13.263	3706	3708	3715	rBV3	189	228	0.01%	0.002%
90	13.848	3885	3890	3896	rVB6	1887	2202	0.14%	0.018%
91	13.880	3896	3900	3903	rBV2	301	262	0.02%	0.002%
92	14.044	3943	3951	3954	rBV3	403	675	0.04%	0.005%
93	14.092	3958	3966	3975	rVV	2425	3756	0.24%	0.030%
94	14.333	4036	4041	4049	rVB5	1588	2101	0.13%	0.017%
95	14.465	4079	4082	4084	rBV2	287	200	0.01%	0.002%
96	14.516	4094	4098	4101	rBV2	310	281	0.02%	0.002%
97	14.918	4221	4223	4227	rBV3	411	273	0.02%	0.002%
98	15.256	4326	4328	4330	rBV	322	218	0.01%	0.002%
99	15.906	4528	4530	4533	rBV3	673	422	0.03%	0.003%
100	16.060	4574	4578	4579	rBV3	633	506	0.03%	0.004%




Sum of corrected areas: 12551472

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047196.D
Acq On : 17 Feb 2022 10:48
Operator : SY/MD
Sample : VU0217WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

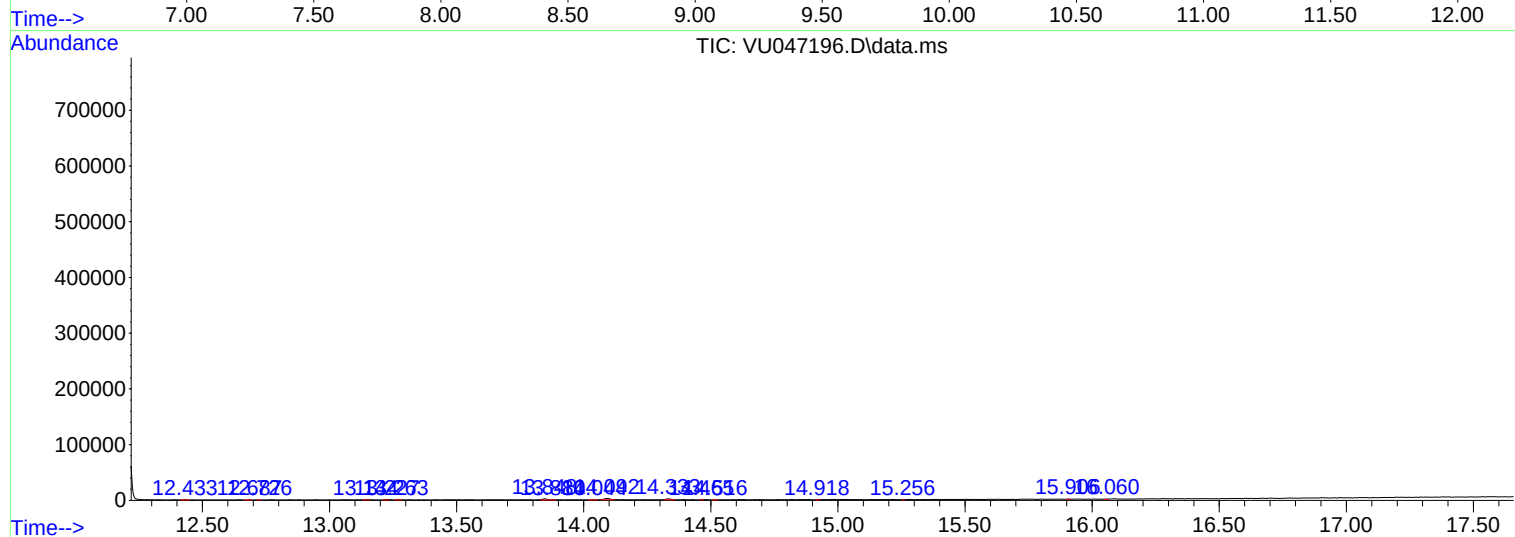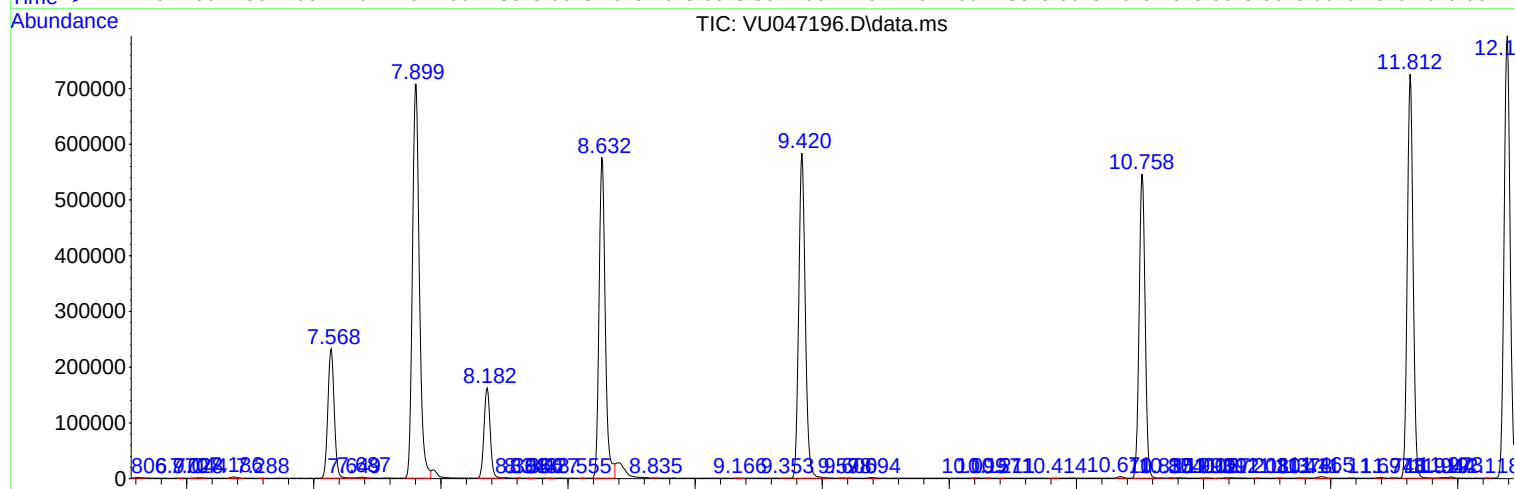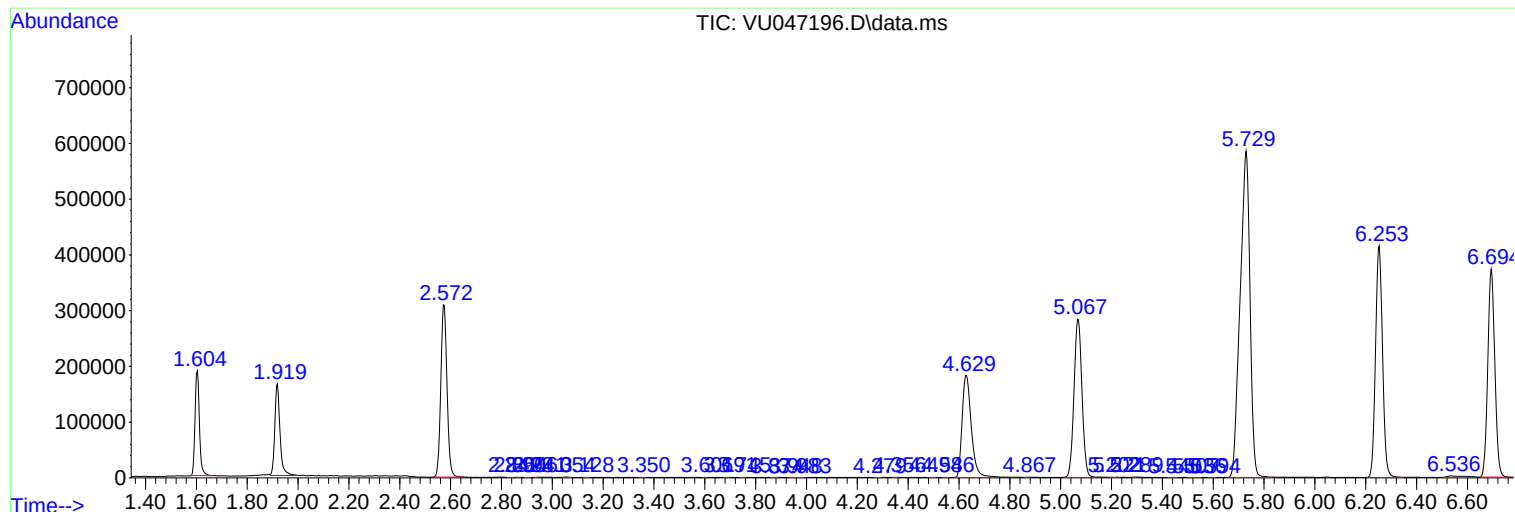

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047196.D
Acq On : 17 Feb 2022 10:48
Operator : SY/MD
Sample : VU0217WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047196.D
Acq On : 17 Feb 2022 10:48
Operator : SY/MD
Sample : VU0217WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc