

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047197.D
 Acq On : 17 Feb 2022 11:13
 Operator : SY/MD
 Sample : N1462-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	103	rVB	197102	235512	14.37%	1.694%
2	1.916	171	179	206	rVB	165979	236817	14.45%	1.703%
3	2.514	362	365	367	rVB2	554	302	0.02%	0.002%
4	2.575	371	384	400	rBV	321832	540534	32.99%	3.888%
5	2.803	440	455	477	rBV5	2840	11667	0.71%	0.084%
6	3.051	528	532	539	rBV3	861	1235	0.08%	0.009%
7	3.298	606	609	615	rVB2	219	242	0.01%	0.002%
8	3.350	619	625	628	rBV3	209	226	0.01%	0.002%
9	3.539	681	684	691	rVB2	283	265	0.02%	0.002%
10	3.658	717	721	724	rBV2	220	216	0.01%	0.002%
11	3.790	755	762	764	rBV2	257	267	0.02%	0.002%
12	4.041	837	840	842	rVB3	252	149	0.01%	0.001%
13	4.057	842	845	850	rVB	241	222	0.01%	0.002%
14	4.154	870	875	878	rBV2	133	155	0.01%	0.001%
15	4.575	1001	1006	1008	rBV4	264	197	0.01%	0.001%
16	4.626	1008	1022	1062	rBV	189112	459089	28.02%	3.302%
17	4.768	1064	1066	1071	rVB3	686	507	0.03%	0.004%
18	5.067	1142	1159	1182	rBV	307290	676880	41.31%	4.868%
19	5.211	1202	1204	1206	rBV	453	224	0.01%	0.002%
20	5.247	1213	1215	1216	rBV	454	216	0.01%	0.002%
21	5.295	1221	1230	1236	rVV4	744	1540	0.09%	0.011%
22	5.363	1248	1251	1254	rVB	345	259	0.02%	0.002%
23	5.572	1311	1316	1318	rBV2	138	150	0.01%	0.001%
24	5.626	1326	1333	1336	rBV	180	262	0.02%	0.002%
25	5.729	1340	1365	1396	rBV2	606038	1638382	100.00%	11.784%
26	6.044	1460	1463	1466	rBV2	451	264	0.02%	0.002%
27	6.112	1480	1484	1485	rBV2	333	207	0.01%	0.001%
28	6.253	1512	1528	1552	rBV	374965	714791	43.63%	5.141%
29	6.379	1563	1567	1570	rBV	223	231	0.01%	0.002%
30	6.436	1582	1585	1594	rBB3	196	221	0.01%	0.002%
31	6.539	1606	1617	1621	rBV6	2304	4177	0.25%	0.030%
32	6.694	1650	1665	1684	rBV	387039	745264	45.49%	5.360%
33	6.800	1688	1698	1710	rVB6	4261	8622	0.53%	0.062%
34	6.935	1734	1740	1741	rBV6	478	406	0.02%	0.003%
35	6.964	1741	1749	1762	rVB5	2535	4648	0.28%	0.033%
36	7.041	1767	1773	1779	rBV6	868	1188	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047197.D
 Acq On : 17 Feb 2022 11:13
 Operator : SY/MD
 Sample : N1462-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	7.189	1810	1819	1827	rBV5	2357	3911	0.24%	0.028%
38	7.353	1867	1870	1872	rBV	242	177	0.01%	0.001%
39	7.407	1880	1887	1888	rBV	334	392	0.02%	0.003%
40	7.456	1900	1902	1907	rVB	267	160	0.01%	0.001%
41	7.568	1923	1937	1956	rBV	241312	414410	25.29%	2.981%
42	7.694	1967	1976	1987	rVB5	2012	3864	0.24%	0.028%
43	7.793	2000	2007	2012	rBV3	455	558	0.03%	0.004%
44	7.899	2026	2040	2053	rBV	754717	1368146	83.51%	9.840%
45	7.973	2053	2063	2095	rVB	696655	1308131	79.84%	9.408%
46	8.182	2115	2128	2147	rBV	165290	277445	16.93%	1.995%
47	8.298	2161	2164	2165	rBV3	261	171	0.01%	0.001%
48	8.420	2196	2202	2203	rBV2	303	259	0.02%	0.002%
49	8.475	2208	2219	2233	rVB2	8183	14646	0.89%	0.105%
50	8.633	2256	2268	2282	rBV	564222	967435	59.05%	6.958%
51	8.899	2347	2351	2356	rBV2	206	245	0.01%	0.002%
52	9.102	2411	2414	2416	rBV3	306	218	0.01%	0.002%
53	9.420	2499	2513	2539	rBV	524496	927500	56.61%	6.671%
54	9.575	2553	2561	2578	rBV4	2114	4662	0.28%	0.034%
55	9.697	2589	2599	2612	rVB2	7440	12784	0.78%	0.092%
56	9.751	2614	2616	2620	rBV3	179	168	0.01%	0.001%
57	9.874	2649	2654	2658	rBV2	192	210	0.01%	0.002%
58	10.012	2694	2697	2700	rVV	244	172	0.01%	0.001%
59	10.083	2710	2719	2740	rBV2	13505	26724	1.63%	0.192%
60	10.231	2761	2765	2768	rBV3	328	337	0.02%	0.002%
61	10.301	2783	2787	2788	rBV	284	161	0.01%	0.001%
62	10.446	2829	2832	2838	rBV3	241	280	0.02%	0.002%
63	10.674	2894	2903	2911	rVB2	3265	5095	0.31%	0.037%
64	10.758	2915	2929	2948	rBV	560103	900166	54.94%	6.474%
65	10.896	2958	2972	2986	rVB	10168	18292	1.12%	0.132%
66	10.999	2998	3004	3006	rBV5	418	426	0.03%	0.003%
67	11.089	3028	3032	3034	rBV2	477	430	0.03%	0.003%
68	11.150	3048	3051	3057	rVB2	620	526	0.03%	0.004%
69	11.298	3094	3097	3102	rVB2	313	304	0.02%	0.002%
70	11.327	3102	3106	3109	rBV3	386	358	0.02%	0.003%
71	11.378	3115	3122	3129	rVB5	755	715	0.04%	0.005%
72	11.459	3138	3147	3149	rBV2	2974	3449	0.21%	0.025%
73	11.616	3193	3196	3206	rBV2	178	227	0.01%	0.002%
74	11.693	3211	3220	3221	rBV3	1503	1542	0.09%	0.011%
75	11.745	3233	3236	3242	rBV4	626	719	0.04%	0.005%
76	11.812	3244	3257	3277	rVV	630978	1013000	61.83%	7.286%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047197.D
 Acq On : 17 Feb 2022 11:13
 Operator : SY/MD
 Sample : N1462-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.941	3292	3297	3302	rBV4	925	1253	0.08%	0.009%
78	11.976	3303	3308	3312	rVB2	1776	2053	0.13%	0.015%
79	12.050	3328	3331	3333	rBV3	329	244	0.01%	0.002%
80	12.195	3358	3376	3395	rVV	823646	1323122	80.76%	9.516%
81	12.301	3407	3409	3413	rVB3	388	219	0.01%	0.002%
82	12.636	3506	3513	3516	rBV4	406	529	0.03%	0.004%
83	12.777	3549	3557	3567	rVB4	2259	3671	0.22%	0.026%
84	12.828	3567	3573	3575	rBV2	267	224	0.01%	0.002%
85	12.864	3579	3584	3586	rBV2	229	231	0.01%	0.002%
86	12.890	3586	3592	3601	rVV7	1820	2544	0.16%	0.018%
87	12.957	3610	3613	3616	rBV	228	152	0.01%	0.001%
88	13.083	3649	3652	3657	rBV2	299	274	0.02%	0.002%
89	13.218	3692	3694	3696	rBV2	364	199	0.01%	0.001%
90	13.295	3715	3718	3721	rBV2	308	161	0.01%	0.001%
91	13.359	3736	3738	3745	rVB3	299	276	0.02%	0.002%
92	13.446	3761	3765	3768	rBV2	337	266	0.02%	0.002%
93	13.726	3848	3852	3858	rBV4	454	674	0.04%	0.005%
94	13.851	3883	3891	3894	rBV3	827	1135	0.07%	0.008%
95	13.967	3923	3927	3931	rBV2	271	287	0.02%	0.002%
96	14.333	4036	4041	4049	rVB5	1038	1435	0.09%	0.010%
97	14.394	4056	4060	4065	rBV2	316	298	0.02%	0.002%
98	14.774	4175	4178	4181	rBV3	313	232	0.01%	0.002%
99	15.423	4378	4380	4384	rBV2	375	242	0.01%	0.002%
100	15.841	4508	4510	4512	rBV2	598	278	0.02%	0.002%




Sum of corrected areas: 13903948

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047197.D
Acq On : 17 Feb 2022 11:13
Operator : SY/MD
Sample : N1462-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

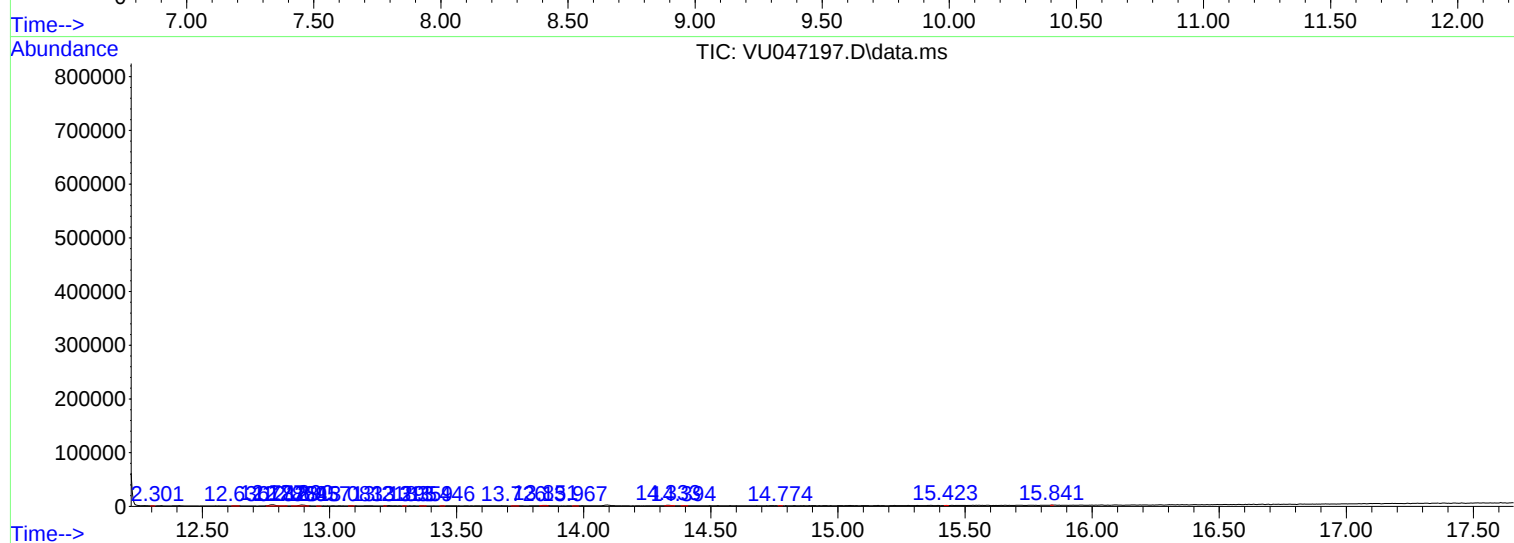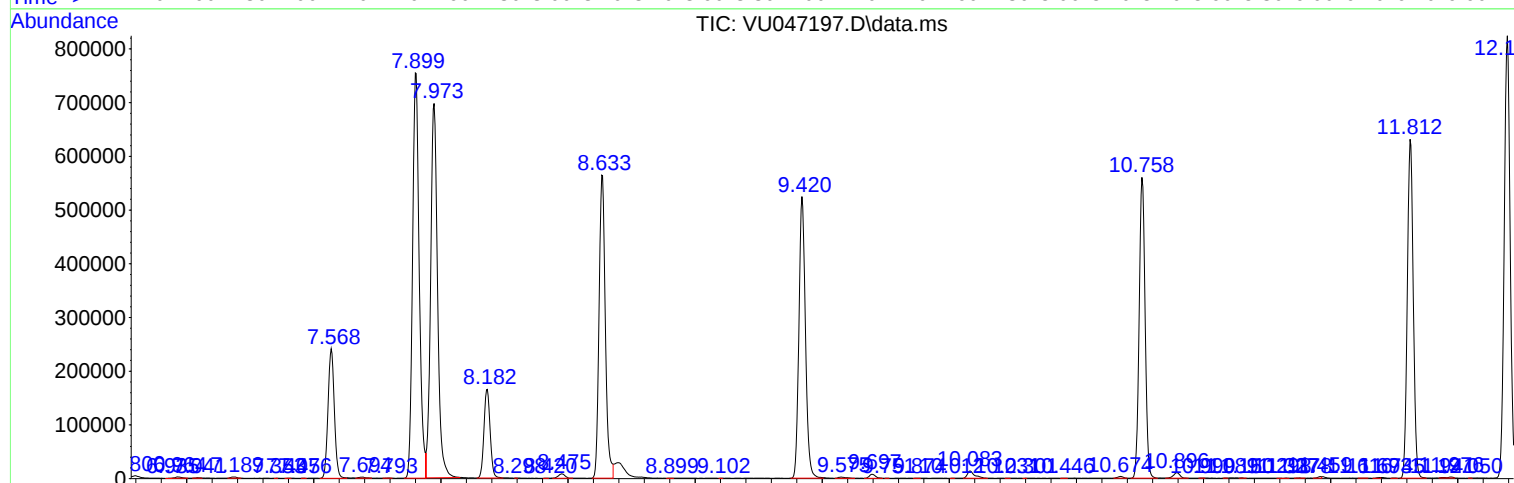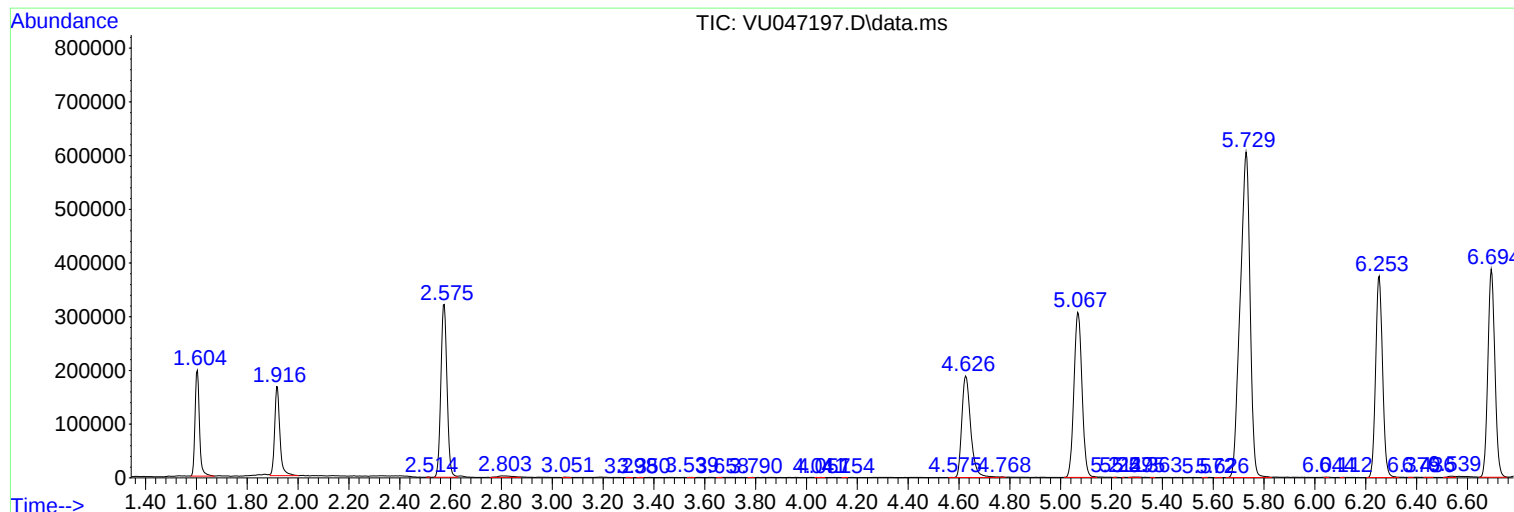

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047197.D
Acq On : 17 Feb 2022 11:13
Operator : SY/MD
Sample : N1462-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047197.D
Acq On : 17 Feb 2022 11:13
Operator : SY/MD
Sample : N1462-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------