

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047198.D
 Acq On : 17 Feb 2022 11:36
 Operator : SY/MD
 Sample : N1462-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M

Title : VOC Analysis

Signal : TIC: VU047198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	178863	211679	14.13%	1.792%
2	1.916	170	179	206	rBV	144107	202995	13.55%	1.718%
3	2.572	370	383	411	rVB	301273	496334	33.13%	4.201%
4	2.675	411	415	417	rBV3	306	192	0.01%	0.002%
5	2.852	468	470	473	rVB2	371	225	0.02%	0.002%
6	2.900	480	485	487	rBV3	310	260	0.02%	0.002%
7	3.054	523	533	539	rBV4	722	1308	0.09%	0.011%
8	3.321	612	616	619	rBV2	234	224	0.01%	0.002%
9	3.376	626	633	636	rBV2	301	291	0.02%	0.002%
10	3.495	667	670	676	rVB2	406	421	0.03%	0.004%
11	3.681	724	728	731	rBV2	284	261	0.02%	0.002%
12	3.723	736	741	744	rVV3	277	262	0.02%	0.002%
13	3.774	751	757	760	rBV3	279	321	0.02%	0.003%
14	3.845	775	779	783	rVV2	355	255	0.02%	0.002%
15	3.916	798	801	807	rVB	296	311	0.02%	0.003%
16	3.948	807	811	814	rBV2	263	262	0.02%	0.002%
17	4.102	855	859	862	rBV3	224	233	0.02%	0.002%
18	4.192	882	887	890	rBV2	244	260	0.02%	0.002%
19	4.241	897	902	904	rBV3	244	285	0.02%	0.002%
20	4.424	956	959	962	rBV2	323	289	0.02%	0.002%
21	4.466	969	972	976	rBV3	284	233	0.02%	0.002%
22	4.623	1007	1021	1054	rVV	178529	423082	28.24%	3.581%
23	5.067	1142	1159	1179	rBV	267589	587117	39.20%	4.970%
24	5.212	1200	1204	1207	rBV2	363	315	0.02%	0.003%
25	5.729	1342	1365	1389	rBV2	550093	1497923	100.00%	12.680%
26	5.919	1421	1424	1434	rVB4	391	410	0.03%	0.003%
27	6.105	1478	1482	1485	rBV	573	468	0.03%	0.004%
28	6.253	1512	1528	1562	rBV	400887	771099	51.48%	6.527%
29	6.536	1606	1616	1621	rBV4	2335	4399	0.29%	0.037%
30	6.694	1650	1665	1692	rVB	356289	684529	45.70%	5.794%
31	6.797	1693	1697	1699	rBV2	502	431	0.03%	0.004%
32	6.967	1747	1750	1754	rBV2	266	233	0.02%	0.002%
33	7.048	1766	1775	1783	rVV4	883	1352	0.09%	0.011%
34	7.122	1794	1798	1804	rVB3	235	212	0.01%	0.002%
35	7.183	1810	1817	1826	rBV4	2564	4206	0.28%	0.036%
36	7.257	1834	1840	1843	rBV3	316	361	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047198.D
 Acq On : 17 Feb 2022 11:36
 Operator : SY/MD
 Sample : N1462-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	7.269	1843	1844	1849	rVB2	365	213	0.01%	0.002%
38	7.411	1885	1888	1891	rBV2	322	305	0.02%	0.003%
39	7.475	1900	1908	1913	rBV3	345	417	0.03%	0.004%
40	7.568	1923	1937	1956	rBV	217728	378230	25.25%	3.202%
41	7.687	1968	1974	1984	rVB7	1587	2789	0.19%	0.024%
42	7.771	1996	2000	2002	rBV2	255	201	0.01%	0.002%
43	7.790	2002	2006	2009	rBV	258	249	0.02%	0.002%
44	7.819	2013	2015	2019	rBV2	262	196	0.01%	0.002%
45	7.900	2026	2040	2060	rBV	679162	1260204	84.13%	10.668%
46	8.183	2114	2128	2149	rBV	151186	251542	16.79%	2.129%
47	8.321	2168	2171	2176	rVB4	313	283	0.02%	0.002%
48	8.404	2194	2197	2199	rVV3	440	215	0.01%	0.002%
49	8.472	2209	2218	2232	rVV	1689	3080	0.21%	0.026%
50	8.633	2256	2268	2282	rBV	537896	894963	59.75%	7.576%
51	8.838	2330	2332	2337	rVB4	364	313	0.02%	0.003%
52	8.909	2351	2354	2360	rBV4	334	415	0.03%	0.004%
53	8.986	2376	2378	2383	rBV3	247	229	0.02%	0.002%
54	9.250	2456	2460	2465	rVB2	299	315	0.02%	0.003%
55	9.420	2500	2513	2547	rBV	558572	996897	66.55%	8.439%
56	9.559	2553	2556	2559	rBV2	311	189	0.01%	0.002%
57	9.578	2559	2562	2567	rVV3	517	403	0.03%	0.003%
58	9.607	2567	2571	2579	rVB4	392	532	0.04%	0.005%
59	9.646	2579	2583	2586	rVB2	269	204	0.01%	0.002%
60	9.697	2591	2599	2606	rBV3	1316	2104	0.14%	0.018%
61	9.726	2606	2608	2618	rVB3	344	412	0.03%	0.003%
62	9.806	2630	2633	2636	rBV3	246	221	0.01%	0.002%
63	9.880	2649	2656	2659	rBV3	274	354	0.02%	0.003%
64	9.938	2670	2674	2679	rBV2	350	381	0.03%	0.003%
65	10.102	2723	2725	2729	rVB3	322	222	0.01%	0.002%
66	10.401	2815	2818	2821	rVB	267	187	0.01%	0.002%
67	10.671	2895	2902	2912	rVB5	2663	4132	0.28%	0.035%
68	10.758	2916	2929	2951	rBV	521564	831306	55.50%	7.037%
69	10.874	2958	2965	2966	rVV4	754	755	0.05%	0.006%
70	10.893	2968	2971	2983	rVB5	2050	2616	0.17%	0.022%
71	11.086	3027	3031	3034	rBV2	249	252	0.02%	0.002%
72	11.115	3037	3040	3047	rBV5	418	521	0.03%	0.004%
73	11.211	3066	3070	3072	rBV2	326	229	0.02%	0.002%
74	11.314	3098	3102	3107	rBV4	269	223	0.01%	0.002%
75	11.414	3130	3133	3137	rVB3	419	278	0.02%	0.002%
76	11.465	3138	3149	3159	rVV6	2390	4671	0.31%	0.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047198.D
 Acq On : 17 Feb 2022 11:36
 Operator : SY/MD
 Sample : N1462-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.575	3179	3183	3188	rBV3	311	373	0.02%	0.003%
78	11.697	3214	3221	3228	rVB5	1331	1906	0.13%	0.016%
79	11.748	3232	3237	3242	rBB4	397	455	0.03%	0.004%
80	11.813	3244	3257	3277	rBV	668835	1066704	71.21%	9.030%
81	11.941	3294	3297	3300	rBV4	786	629	0.04%	0.005%
82	12.195	3358	3376	3392	rBV	741521	1202880	80.30%	10.182%
83	12.334	3415	3419	3424	rVB3	656	541	0.04%	0.005%
84	12.642	3512	3515	3521	rVB3	486	389	0.03%	0.003%
85	12.710	3530	3536	3538	rBV2	265	322	0.02%	0.003%
86	12.758	3547	3551	3553	rBV	424	346	0.02%	0.003%
87	13.221	3692	3695	3701	rVB2	343	349	0.02%	0.003%
88	13.298	3715	3719	3720	rBV2	272	210	0.01%	0.002%
89	13.330	3726	3729	3734	rVB3	405	255	0.02%	0.002%
90	13.555	3797	3799	3802	rBV3	353	244	0.02%	0.002%
91	13.665	3830	3833	3835	rBV2	380	250	0.02%	0.002%
92	13.845	3884	3889	3891	rBV5	738	761	0.05%	0.006%
93	14.096	3963	3967	3970	rBV	661	484	0.03%	0.004%
94	14.478	4083	4086	4088	rBV2	331	246	0.02%	0.002%
95	14.604	4122	4125	4130	rVB3	306	271	0.02%	0.002%
96	14.951	4230	4233	4234	rBV	329	216	0.01%	0.002%
97	14.999	4246	4248	4250	rBV2	373	223	0.01%	0.002%
98	15.163	4297	4299	4304	rBB2	393	285	0.02%	0.002%
99	15.530	4411	4413	4417	rBV3	491	349	0.02%	0.003%
100	15.632	4443	4445	4452	rBV4	481	481	0.03%	0.004%




Sum of corrected areas: 11813455

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047198.D
Acq On : 17 Feb 2022 11:36
Operator : SY/MD
Sample : N1462-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

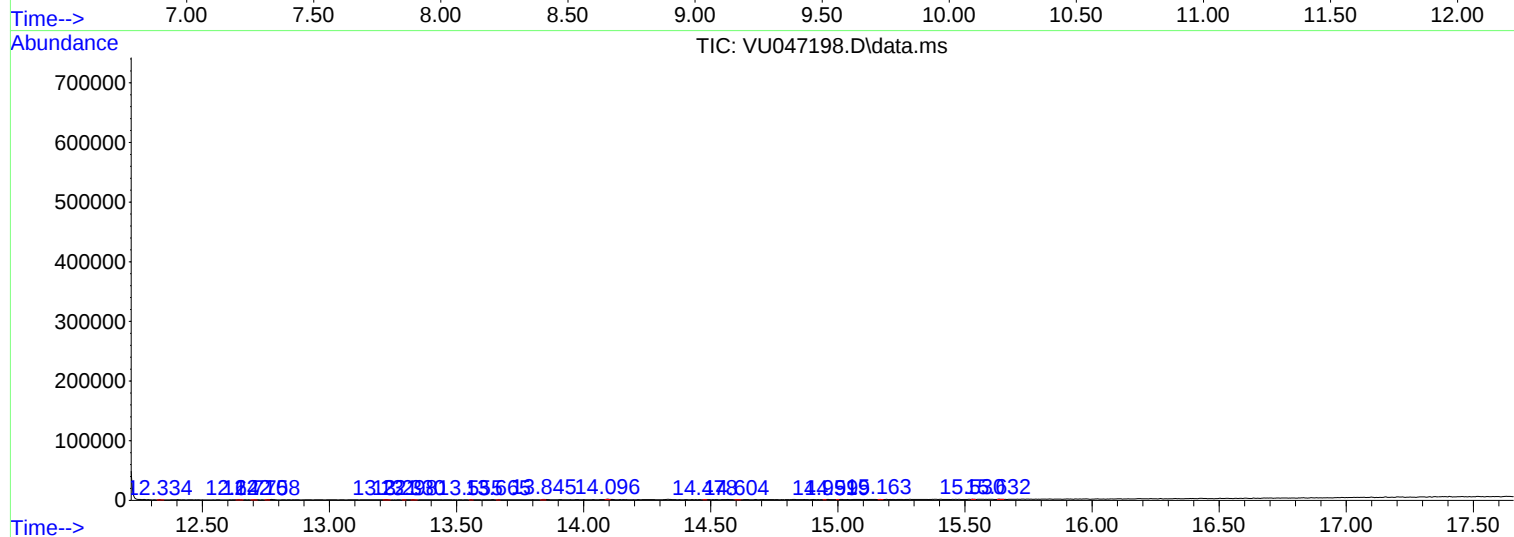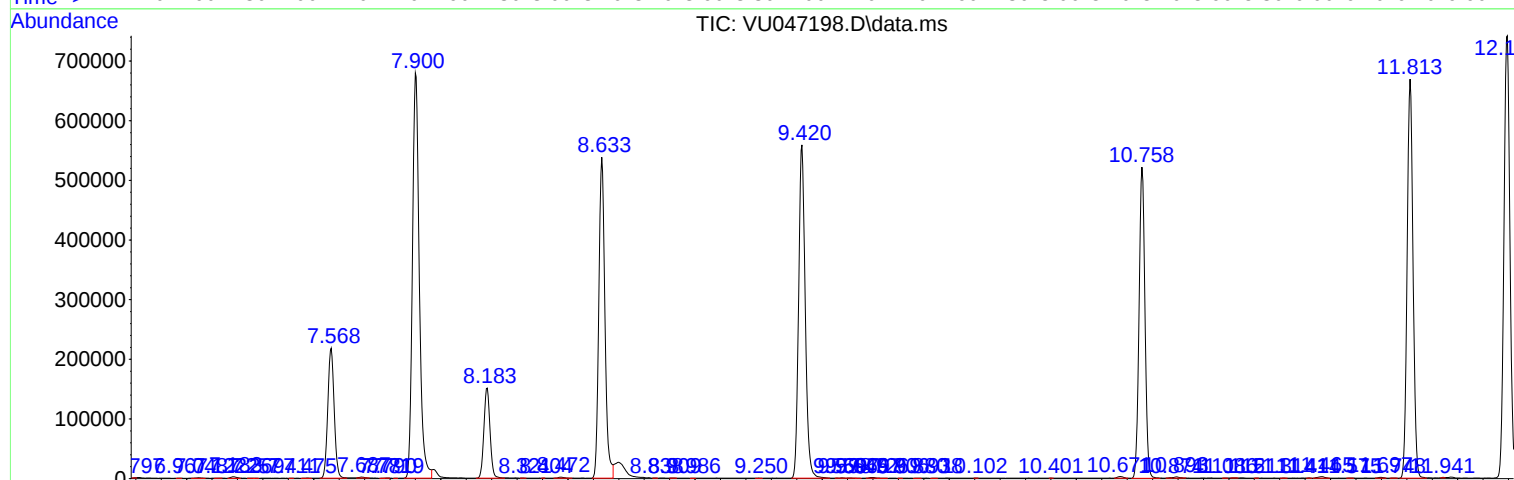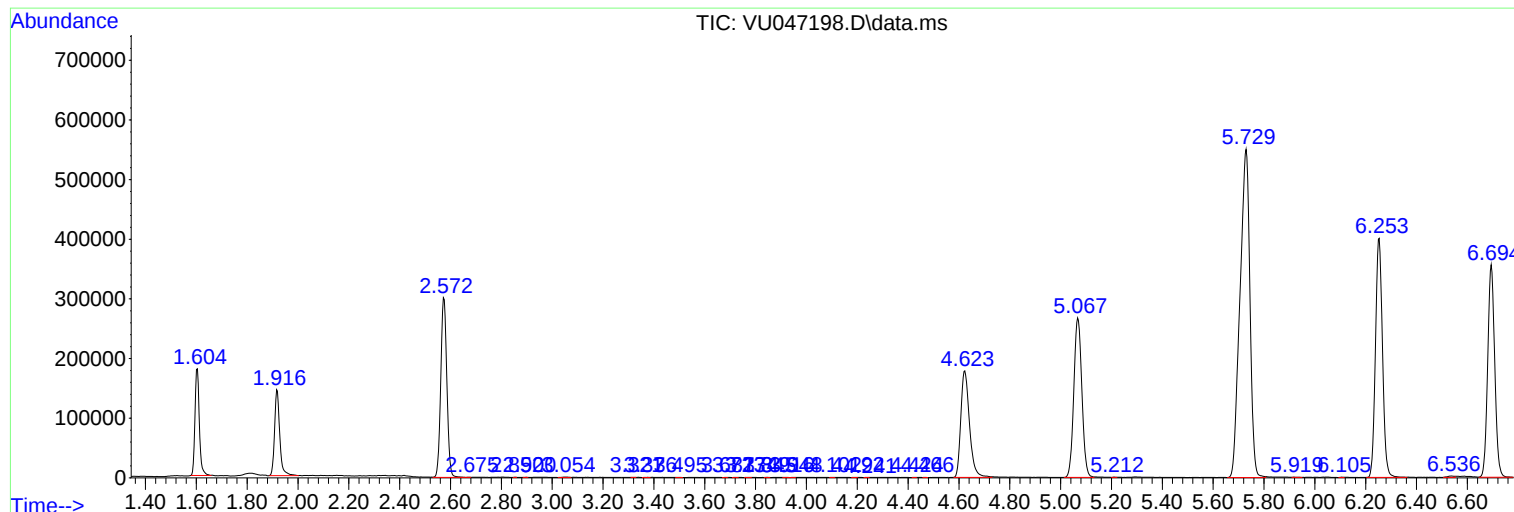

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047198.D
Acq On : 17 Feb 2022 11:36
Operator : SY/MD
Sample : N1462-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047198.D
Acq On : 17 Feb 2022 11:36
Operator : SY/MD
Sample : N1462-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------