

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047200.D
 Acq On : 17 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1474-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M

Title : VOC Analysis

Signal : TIC: VU047200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	103	rBV	191021	229712	14.04%	1.767%
2	1.919	171	180	203	rVB	169642	236282	14.44%	1.818%
3	2.376	320	322	327	rBV5	1016	878	0.05%	0.007%
4	2.572	370	383	416	rVB	321501	540718	33.04%	4.160%
5	2.961	496	504	507	rBV3	635	854	0.05%	0.007%
6	3.009	516	519	525	rVB3	422	287	0.02%	0.002%
7	3.051	525	532	537	rBV3	719	959	0.06%	0.007%
8	3.244	584	592	595	rBV2	198	257	0.02%	0.002%
9	3.353	623	626	630	rBV2	292	218	0.01%	0.002%
10	3.376	630	633	636	rBV	423	235	0.01%	0.002%
11	3.964	811	816	818	rBV3	183	191	0.01%	0.001%
12	4.019	827	833	836	rBV3	185	202	0.01%	0.002%
13	4.067	845	848	853	rVV3	191	196	0.01%	0.002%
14	4.170	875	880	883	rVB3	252	283	0.02%	0.002%
15	4.192	883	887	890	rBV2	198	187	0.01%	0.001%
16	4.482	973	977	983	rBV2	297	361	0.02%	0.003%
17	4.629	1006	1023	1061	rBV	192378	485109	29.64%	3.732%
18	4.855	1090	1093	1096	rVB3	351	234	0.01%	0.002%
19	4.880	1098	1101	1107	rVB2	312	314	0.02%	0.002%
20	5.067	1142	1159	1183	rBV	291852	642317	39.24%	4.942%
21	5.559	1309	1312	1315	rBV	279	199	0.01%	0.002%
22	5.610	1324	1328	1333	rBV2	204	231	0.01%	0.002%
23	5.729	1336	1365	1394	rBV2	607141	1636699	100.00%	12.592%
24	6.044	1457	1463	1471	rVB4	576	1050	0.06%	0.008%
25	6.134	1489	1491	1496	rVB4	302	194	0.01%	0.001%
26	6.253	1511	1528	1557	rBV	427306	822001	50.22%	6.324%
27	6.536	1607	1616	1622	rBV6	2564	5532	0.34%	0.043%
28	6.694	1650	1665	1687	rBV	383437	740900	45.27%	5.700%
29	6.858	1714	1716	1719	rVB2	516	314	0.02%	0.002%
30	6.880	1719	1723	1725	rBV2	276	192	0.01%	0.001%
31	6.961	1741	1748	1751	rBV3	351	371	0.02%	0.003%
32	6.980	1751	1754	1758	rVB	288	229	0.01%	0.002%
33	7.009	1758	1763	1766	rBV2	356	287	0.02%	0.002%
34	7.041	1766	1773	1775	rBV2	851	849	0.05%	0.007%
35	7.182	1810	1817	1829	rBV5	2767	4597	0.28%	0.035%
36	7.237	1832	1834	1843	rVB3	355	372	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047200.D
 Acq On : 17 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1474-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	7.388	1879	1881	1885	rVB2	302	216	0.01%	0.002%
38	7.417	1885	1890	1893	rBV2	312	347	0.02%	0.003%
39	7.568	1923	1937	1956	rBV	236889	413249	25.25%	3.179%
40	7.687	1970	1974	1986	rVB3	1921	2986	0.18%	0.023%
41	7.764	1995	1998	2002	rVB	237	197	0.01%	0.002%
42	7.790	2002	2006	2010	rBV3	247	298	0.02%	0.002%
43	7.903	2025	2041	2060	rBV	736366	1382277	84.46%	10.635%
44	8.182	2113	2128	2146	rBV	162701	276574	16.90%	2.128%
45	8.305	2164	2166	2170	rVB3	353	179	0.01%	0.001%
46	8.385	2186	2191	2196	rVB4	281	301	0.02%	0.002%
47	8.475	2210	2219	2230	rVB4	1508	2672	0.16%	0.021%
48	8.571	2246	2249	2251	rVB2	321	206	0.01%	0.002%
49	8.633	2255	2268	2282	rBV	595233	1014239	61.97%	7.803%
50	8.919	2353	2357	2360	rVB2	474	460	0.03%	0.004%
51	8.993	2376	2380	2384	rBV2	340	342	0.02%	0.003%
52	9.128	2417	2422	2430	rBV3	312	522	0.03%	0.004%
53	9.340	2483	2488	2495	rBV2	213	232	0.01%	0.002%
54	9.420	2499	2513	2550	rVB	611385	1075651	65.72%	8.276%
55	9.571	2556	2560	2564	rBV3	215	254	0.02%	0.002%
56	9.597	2566	2568	2574	rVB2	275	220	0.01%	0.002%
57	9.697	2590	2599	2606	rBV4	1294	1769	0.11%	0.014%
58	10.259	2769	2774	2777	rBV3	260	314	0.02%	0.002%
59	10.478	2840	2842	2847	rVB2	262	244	0.01%	0.002%
60	10.526	2854	2857	2862	rVB3	307	214	0.01%	0.002%
61	10.623	2879	2887	2889	rBV2	279	283	0.02%	0.002%
62	10.674	2894	2903	2911	rVB2	3402	4968	0.30%	0.038%
63	10.758	2916	2929	2949	rBV	566032	917664	56.07%	7.060%
64	10.893	2963	2971	2982	rVB5	1622	2999	0.18%	0.023%
65	10.996	3000	3003	3005	rBV2	254	206	0.01%	0.002%
66	11.095	3032	3034	3037	rVV2	493	359	0.02%	0.003%
67	11.118	3037	3041	3046	rVV4	754	967	0.06%	0.007%
68	11.153	3049	3052	3058	rVV4	513	506	0.03%	0.004%
69	11.205	3062	3068	3073	rVB5	469	528	0.03%	0.004%
70	11.237	3073	3078	3082	rBV2	245	242	0.01%	0.002%
71	11.298	3092	3097	3102	rBV3	343	474	0.03%	0.004%
72	11.330	3104	3107	3110	rVB3	374	317	0.02%	0.002%
73	11.465	3138	3149	3161	rBV6	2921	5370	0.33%	0.041%
74	11.578	3180	3184	3190	rVB4	600	651	0.04%	0.005%
75	11.697	3215	3221	3228	rVV3	1614	2224	0.14%	0.017%
76	11.745	3232	3236	3239	rVB3	210	193	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047200.D
 Acq On : 17 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1474-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.812	3244	3257	3274	rBV	737367	1171914	71.60%	9.016%
78	11.944	3291	3298	3301	rBV5	1347	1784	0.11%	0.014%
79	11.970	3303	3306	3315	rVB5	2348	3042	0.19%	0.023%
80	12.012	3315	3319	3322	rBV3	344	322	0.02%	0.002%
81	12.111	3347	3350	3353	rVB2	331	230	0.01%	0.002%
82	12.195	3360	3376	3393	rBV	830807	1346794	82.29%	10.362%
83	12.330	3412	3418	3424	rBV5	1157	1307	0.08%	0.010%
84	12.594	3495	3500	3503	rBV3	338	300	0.02%	0.002%
85	12.632	3508	3512	3513	rBV2	259	193	0.01%	0.001%
86	12.758	3546	3551	3553	rBV3	437	346	0.02%	0.003%
87	12.780	3554	3558	3562	rVB2	545	554	0.03%	0.004%
88	13.092	3650	3655	3658	rBV2	245	206	0.01%	0.002%
89	13.430	3754	3760	3764	rBV3	419	496	0.03%	0.004%
90	13.520	3783	3788	3791	rBV	438	361	0.02%	0.003%
91	13.851	3885	3891	3897	rBV3	514	775	0.05%	0.006%
92	13.960	3920	3925	3927	rBV2	312	314	0.02%	0.002%
93	14.057	3950	3955	3959	rBV2	467	433	0.03%	0.003%
94	14.086	3960	3964	3965	rBV2	420	307	0.02%	0.002%
95	14.282	4020	4025	4027	rBV2	446	357	0.02%	0.003%
96	14.381	4052	4056	4059	rBV3	333	297	0.02%	0.002%
97	14.574	4113	4116	4122	rBV3	414	321	0.02%	0.002%
98	14.848	4199	4201	4207	rVB4	532	581	0.04%	0.004%
99	14.877	4207	4210	4213	rBV2	385	321	0.02%	0.002%
100	15.336	4350	4353	4354	rBV3	349	195	0.01%	0.002%




Sum of corrected areas: 12997475

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047200.D
Acq On : 17 Feb 2022 12:23
Operator : SY/MD
Sample : N1474-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

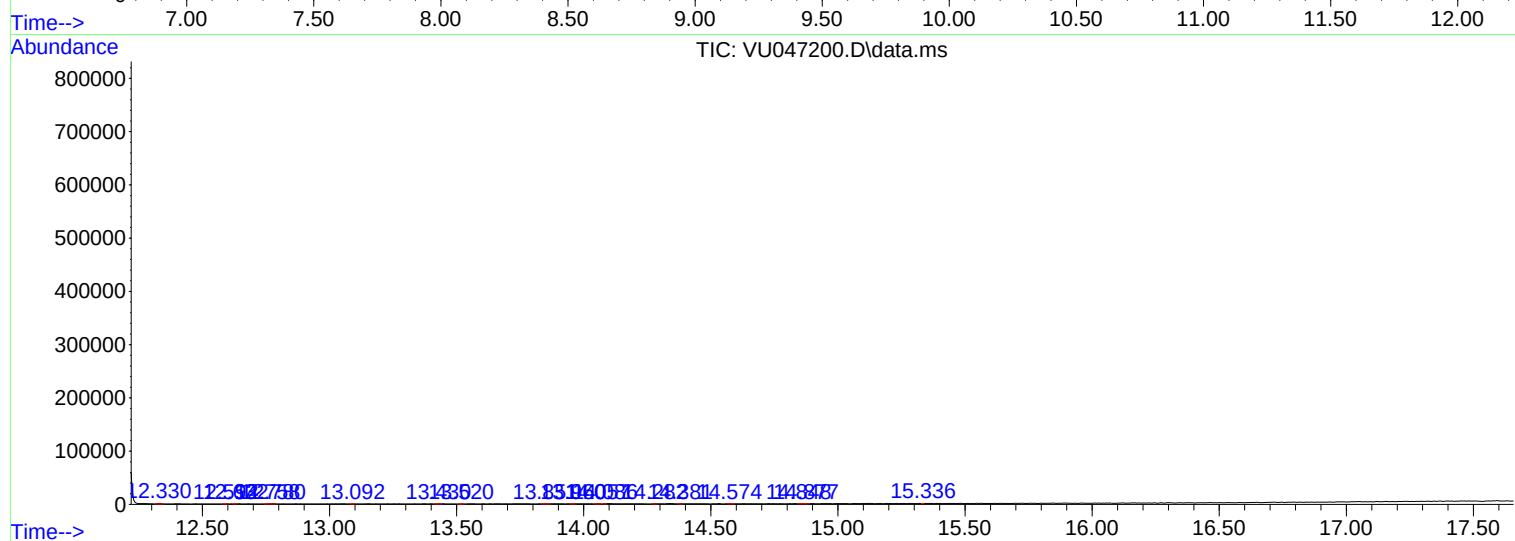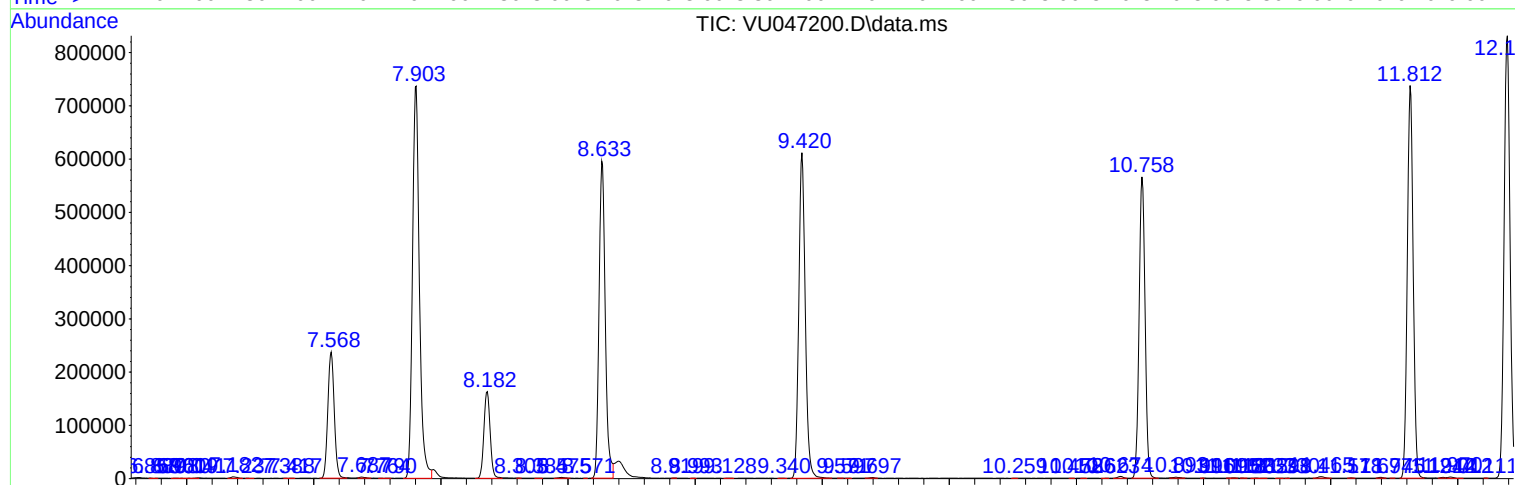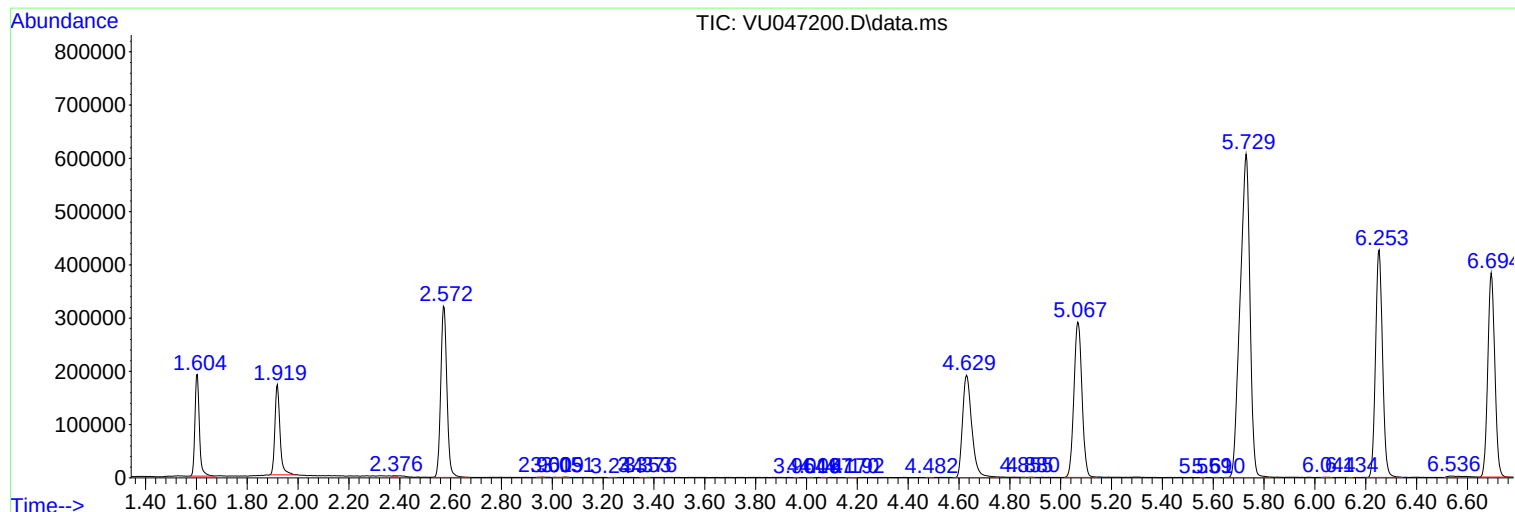

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047200.D
Acq On : 17 Feb 2022 12:23
Operator : SY/MD
Sample : N1474-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
Data File : VU047200.D
Acq On : 17 Feb 2022 12:23
Operator : SY/MD
Sample : N1474-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc