


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021722\
 Data File : VU047193.D
 Acq On : 17 Feb 2022 08:57
 Operator : SY/MD
 Sample : BFB045
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB045

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis
 Last Update : Fri Feb 18 00:54:38 2022

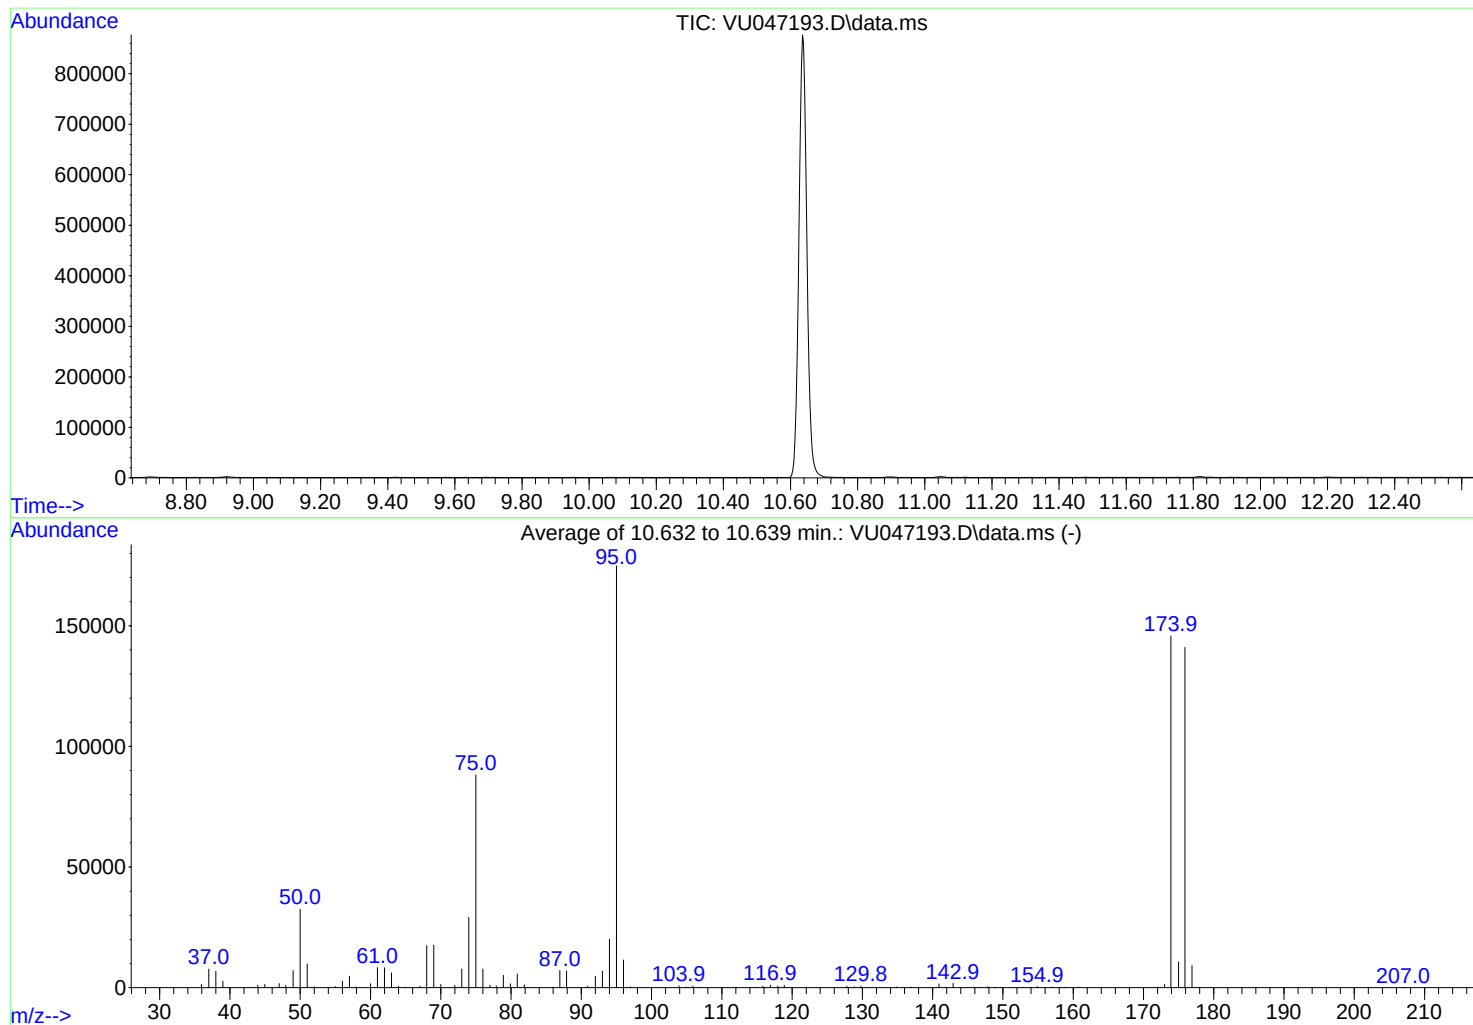

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	32496	PASS
75	95	30	80	50.5	88229	PASS
95	95	100	100	100.0	174869	PASS
96	95	5	9	6.6	11491	PASS
173	174	0.00	2	0.9	1303	PASS
174	95	50	120	83.4	145792	PASS
175	174	5	9	7.3	10705	PASS
176	174	95	101	96.8	141120	PASS
177	176	5	9	6.5	9174	PASS

Scan 2877 (10.591 min): VU047193.D\data.ms
BFB045

m/z	Abundance
39.80	111.0
43.80	379.0
207.00	217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
36.00	1356.0
37.00	7536.0
38.00	6601.0
39.00	2727.0
39.90	220.0
43.00	140.0
44.00	1406.0
45.00	1376.0
47.00	1568.0
47.90	905.0
49.00	6974.0
50.00	31744.0
51.00	9634.0
52.00	307.0
55.00	400.0
56.00	2752.0
57.00	4540.0
57.90	254.0
60.00	1526.0
61.00	8035.0
62.00	8084.0
63.00	6003.0
64.00	583.0
65.00	184.0
67.00	477.0
68.00	16840.0
69.00	17264.0
70.00	1337.0
72.00	933.0
73.00	7538.0
74.00	28064.0
75.00	84968.0
76.00	7711.0
77.00	970.0
77.90	673.0
78.90	4941.0
79.90	1515.0
80.90	5579.0
81.90	1090.0
82.90	126.0
86.00	199.0
87.00	6995.0
87.90	6747.0
90.90	649.0
92.00	4403.0
93.00	6635.0
94.00	19416.0
95.00	168064.0
96.00	11108.0
97.00	293.0
103.90	710.0
104.90	301.0
105.90	727.0
106.80	151.0
109.80	112.0
110.90	139.0
114.80	181.0
115.90	596.0
116.90	987.0
117.90	503.0
118.90	913.0
123.80	127.0
127.80	520.0
128.90	286.0
129.80	539.0
131.00	200.0
134.80	214.0
136.90	290.0
139.80	134.0
140.90	1489.0
141.80	181.0
142.90	1664.0
143.90	121.0
144.90	159.0
145.90	292.0
146.80	103.0
147.90	418.0
149.80	140.0
152.90	140.0
153.90	116.0
154.90	319.0
157.00	277.0
158.80	181.0
160.70	177.0
172.00	219.0
173.00	1204.0
173.90	137600.0
175.00	10471.0
175.90	132096.0
176.90	8752.0
177.90	219.0
207.00	252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	1403.0
37.00	7979.0
38.00	6995.0
39.00	2752.0
40.00	219.0
43.00	143.0
44.00	1413.0
45.00	1365.0
47.00	1707.0
48.00	995.0
49.00	7354.0
50.00	33648.0
51.00	10164.0
52.00	341.0
55.00	452.0
56.00	2767.0
57.00	4881.0
58.00	252.0
60.00	1673.0
61.00	8565.0
62.00	8448.0
63.00	6301.0
64.00	649.0
65.00	187.0
67.00	521.0
68.00	18120.0
69.00	18128.0
70.00	1412.0
72.00	944.0
73.00	8086.0
74.00	30072.0
75.00	91368.0
76.00	8024.0
77.00	1101.0
77.90	754.0
78.90	5227.0
79.90	1649.0
80.90	5808.0
81.90	1158.0
82.90	112.0
85.90	212.0
86.90	7322.0
87.90	7129.0
90.90	666.0
92.00	4856.0
93.00	6972.0
94.00	20656.0
95.00	180224.0
96.00	11881.0
97.00	337.0
103.90	728.0
104.90	305.0
105.90	726.0
106.90	168.0
109.90	111.0
110.90	153.0
112.00	102.0
114.90	196.0
115.80	606.0
116.90	1085.0
118.00	624.0
118.90	937.0
123.80	155.0
127.80	607.0
128.80	306.0
129.80	625.0
131.00	239.0
134.90	250.0
136.90	314.0
139.80	154.0
140.90	1615.0
141.90	177.0
142.90	1779.0
143.90	119.0
144.90	178.0
145.90	310.0
146.80	110.0
147.90	422.0
148.80	106.0
149.90	145.0
152.90	142.0
153.90	120.0
154.90	385.0
157.00	286.0
158.80	201.0
160.80	173.0
172.00	261.0
173.00	1360.0
173.90	150464.0
175.00	11039.0
175.90	145408.0
176.90	9423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

177.90207.00

256.0228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.00	1300.0
37.00	7663.0
38.00	6745.0
39.00	2637.0
40.00	210.0
43.00	133.0
44.00	1358.0
44.90	1319.0
47.00	1706.0
48.00	955.0
49.00	7035.0
50.00	32096.0
51.00	9687.0
52.00	337.0
55.00	500.0
56.00	2539.0
57.00	4819.0
58.00	221.0
60.00	1599.0
61.00	8288.0
62.00	8101.0
63.00	6051.0
64.00	618.0
64.90	141.0
67.10	555.0
68.00	17448.0
69.00	17424.0
70.00	1342.0
72.00	880.0
73.00	7769.0
74.00	29224.0
75.00	88352.0
76.00	7466.0
77.00	1136.0
77.90	740.0
78.90	5104.0
79.90	1597.0
80.90	5543.0
81.90	1140.0
86.00	196.0
86.90	7059.0
87.90	6873.0
90.90	567.0
92.00	4847.0
93.00	6832.0
94.00	20304.0
95.00	176320.0
96.00	11483.0
97.00	363.0
103.90	726.0
104.90	257.0
105.90	677.0
106.80	167.0
109.90	100.0
110.90	145.0
114.90	201.0
115.80	582.0
116.90	1082.0
117.90	692.0
118.90	873.0
123.80	133.0
127.80	637.0
128.80	319.0
129.80	651.0
130.90	257.0
134.90	285.0
136.90	295.0
139.80	134.0
140.90	1593.0
141.90	153.0
142.90	1730.0
143.90	111.0
144.90	162.0
145.90	299.0
146.80	111.0
147.80	373.0
149.90	154.0
152.90	118.0
153.80	116.0
154.90	407.0
156.90	273.0
158.90	203.0
160.80	175.0
172.00	288.0
173.00	1346.0
173.90	149312.0
175.00	10605.0
175.90	145856.0
176.90	9348.0
177.90	250.0
207.00	251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045