


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021723\
Data File : VU053119.D
Acq On : 17 Feb 2023 09:04
Operator : JC/MD
Sample : BFB161
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB161

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021423WMA.M
Title : VOC Analysis
Last Update : Fri Feb 17 11:12:12 2023

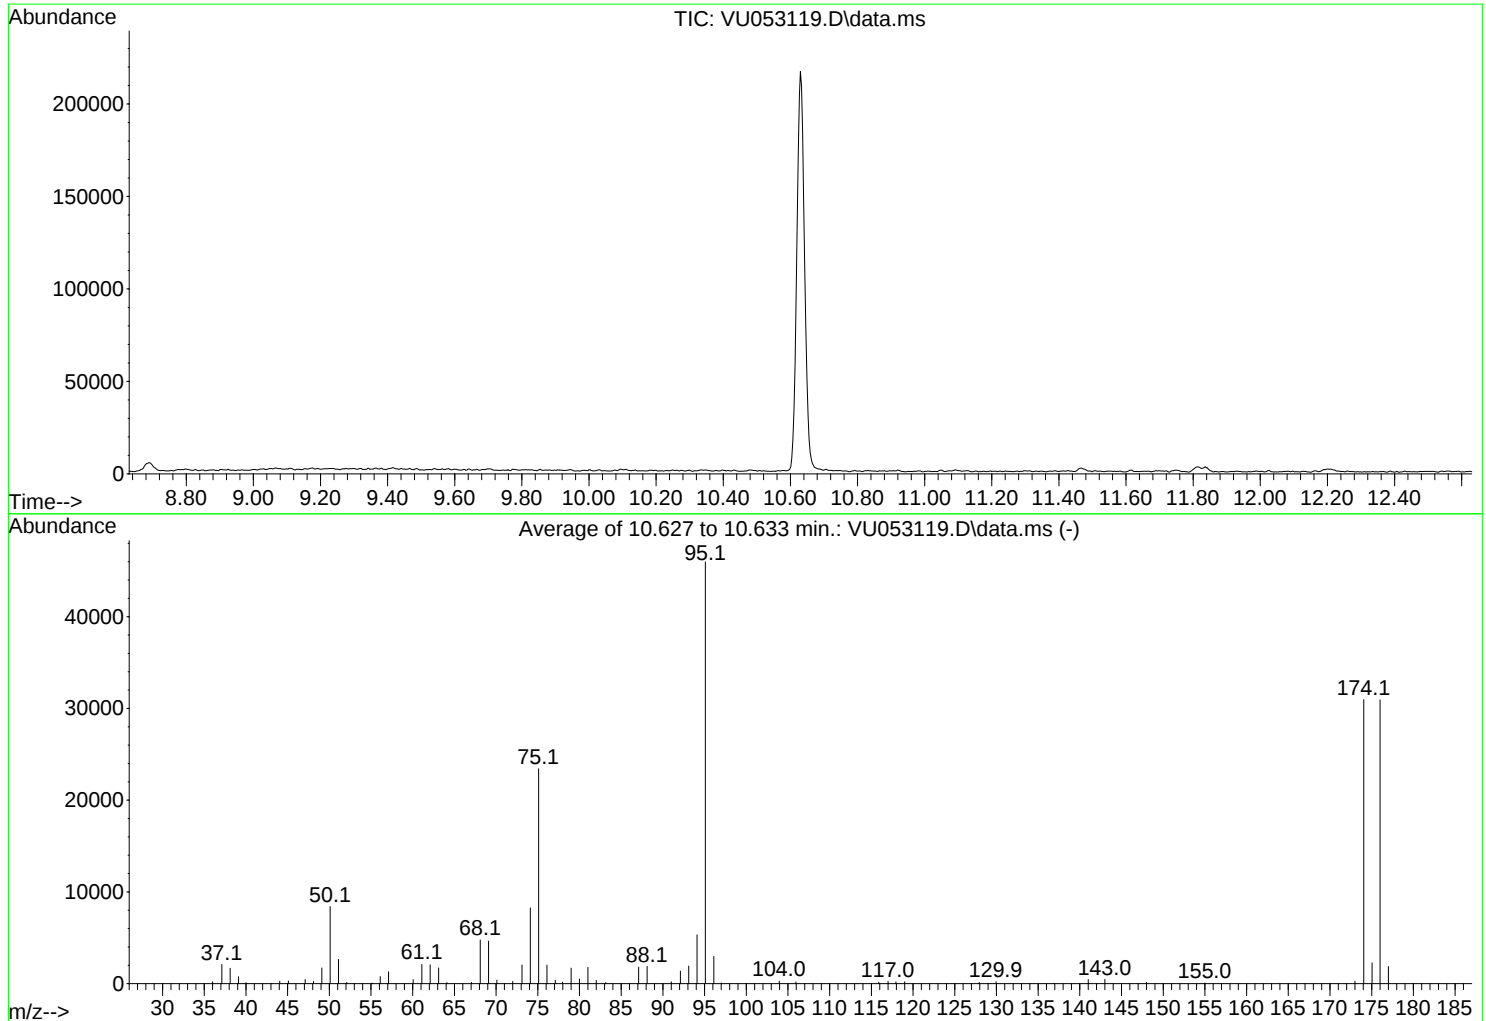

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2954

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	8417	PASS
75	95	30	80	51.0	23427	PASS
95	95	100	100	100.0	45979	PASS
96	95	5	9	6.4	2960	PASS
173	174	0.00	2	0.9	268	PASS
174	95	50	120	67.3	30955	PASS
175	174	5	9	7.3	2268	PASS
176	174	95	101	100.0	30949	PASS
177	176	5	9	6.0	1866	PASS

m/z	Abundance
35.10	126.0
36.00	804.0
38.10	226.0
41.10	153.0
44.00	266.0
55.10	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB161

m/z	Abundance
36.00	1042.0
37.10	2033.0
38.10	1862.0
39.10	690.0
40.00	109.0
41.20	126.0
43.10	107.0
44.10	485.0
45.10	316.0
47.10	464.0
48.10	253.0
49.10	1660.0
50.10	8280.0
51.10	2733.0
52.10	147.0
55.20	164.0
56.10	705.0
57.10	1262.0
60.10	444.0
61.10	2071.0
62.10	1942.0
63.10	1599.0
64.10	132.0
67.10	113.0
68.10	4730.0
69.10	4535.0
70.10	347.0
72.00	232.0
73.10	1941.0
74.10	8006.0
75.10	22656.0
76.10	1977.0
77.10	363.0
77.90	170.0
79.00	1735.0
80.00	528.0
81.00	1759.0
82.00	329.0
83.10	113.0
87.10	1807.0
88.10	1733.0
91.00	259.0
92.10	1291.0
93.10	1916.0
94.10	5281.0
95.10	45280.0
96.10	2995.0
97.00	114.0
103.90	238.0
105.90	219.0
115.90	144.0
117.00	217.0
117.90	179.0
119.00	198.0
128.00	176.0
130.00	189.0
141.00	496.0
143.00	477.0
148.00	124.0
173.10	264.0
174.00	29360.0
175.00	2243.0
176.00	29800.0
177.00	1877.0

Instrument :
MSVOA_U
ClientSampleId :
BFB161

m/z	Abundance
36.00	1014.0
37.10	2164.0
38.10	1977.0
39.10	782.0
40.00	102.0
44.10	563.0
45.10	304.0
47.10	467.0
48.10	269.0
49.10	1757.0
50.10	8716.0
51.10	2762.0
52.10	153.0
55.20	176.0
56.10	792.0
57.10	1324.0
60.00	460.0
61.10	2199.0
62.10	2096.0
63.10	1793.0
64.10	127.0
67.00	142.0
68.10	4930.0
69.10	4765.0
70.10	383.0
72.00	259.0
73.10	2104.0
74.10	8560.0
75.10	24272.0
76.10	2092.0
77.10	416.0
78.00	168.0
79.00	1730.0
80.00	532.0
81.00	1833.0
82.00	363.0
83.10	125.0
87.10	1905.0
88.10	1941.0
91.00	225.0
92.10	1401.0
93.10	1980.0
94.10	5478.0
95.10	47480.0
96.10	3048.0
97.00	123.0
104.00	278.0
105.90	190.0
115.90	187.0
117.00	244.0
118.00	217.0
119.00	225.0
127.90	145.0
130.00	223.0
136.90	101.0
141.00	468.0
143.00	486.0
148.00	151.0
155.00	108.0
173.00	269.0
174.00	31688.0
175.10	2353.0
176.00	31920.0
177.00	1923.0

Instrument :
MSVOA_U
ClientSampleId :
BFB161

m/z	Abundance
36.10	985.0
37.10	2062.0
38.10	1866.0
39.10	783.0
40.00	103.0
44.10	595.0
45.10	274.0
47.10	415.0
48.10	227.0
49.10	1719.0
50.10	8254.0
51.10	2440.0
52.10	123.0
55.20	204.0
56.10	823.0
57.10	1274.0
60.00	392.0
61.10	2032.0
62.10	2140.0
63.10	1754.0
64.10	113.0
67.00	145.0
68.10	4618.0
69.10	4642.0
70.10	408.0
72.00	260.0
73.10	2060.0
74.10	8173.0
75.10	23352.0
76.10	2031.0
77.10	364.0
78.00	194.0
79.00	1634.0
80.00	457.0
81.00	1772.0
82.00	374.0
83.20	115.0
87.10	1664.0
88.10	1965.0
91.00	169.0
92.10	1395.0
93.10	1886.0
94.10	5216.0
95.10	45176.0
96.10	2837.0
104.00	299.0
106.00	163.0
115.90	165.0
117.00	259.0
118.00	215.0
119.00	206.0
128.00	110.0
129.00	108.0
129.90	229.0
141.00	406.0
143.00	439.0
148.00	145.0
155.00	108.0
172.90	272.0
174.10	31816.0
175.00	2209.0
176.00	31128.0
177.00	1798.0

Instrument :
MSVOA_U
ClientSampleId :
BFB161