


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU021819\
Data File : VU029517.D
Acq On : 18 Feb 2019 09:13
Operator : JC/SP
Sample : BFB44
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Feb 19 00:19:12 2019

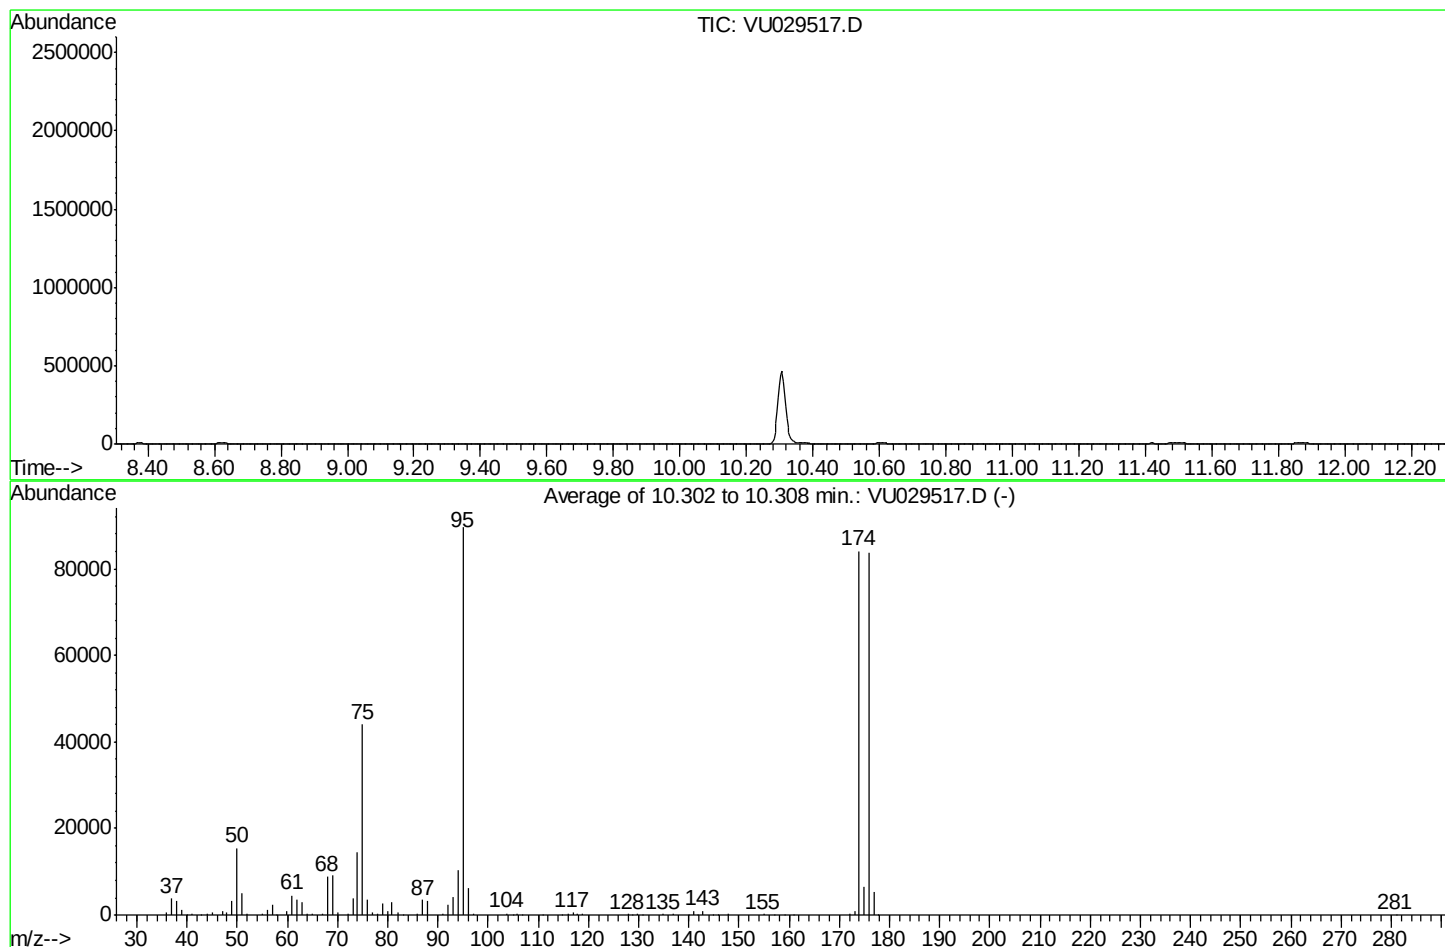

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	15492	PASS
75	95	30	80	49.1	43984	PASS
95	95	100	100	100.0	89570	PASS
96	95	5	9	6.8	6092	PASS
173	174	0.00	2	1.2	979	PASS
174	95	50	120	93.9	84106	PASS
175	174	5	9	7.7	6449	PASS
176	174	95	101	99.4	83640	PASS
177	176	5	9	6.3	5251	PASS

Scan 2852 (10.260 min): VU029517.D
BFB44

m/z	Abundance
40.00	233.0
43.90	580.0
207.00	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	692.0
37.00	3738.0
38.00	3253.0
39.00	1279.0
40.00	339.0
41.00	131.0
42.80	135.0
44.00	902.0
45.00	722.0
47.00	846.0
48.00	560.0
49.00	3399.0
50.00	15579.0
51.00	4875.0
52.00	192.0
55.10	360.0
56.00	1242.0
57.00	2341.0
57.90	123.0
59.90	710.0
61.00	4389.0
62.00	3513.0
63.00	2870.0
63.90	256.0
65.00	148.0
66.90	231.0
68.00	8484.0
69.00	9379.0
70.00	614.0
72.00	406.0
73.00	3545.0
74.00	14704.0
75.00	43104.0
76.00	3704.0
76.90	593.0
78.00	364.0
78.90	2882.0
79.90	835.0
80.90	2870.0
81.90	579.0
83.10	117.0
85.90	135.0
87.00	3402.0
88.00	3311.0
90.90	338.0
92.00	2201.0
93.00	4019.0
94.00	10285.0
95.00	87992.0
96.10	6113.0
97.00	243.0
103.90	379.0
105.00	156.0
105.90	310.0
106.90	120.0
110.90	150.0
114.80	122.0
115.90	396.0
116.80	531.0
117.90	323.0
118.90	427.0
128.00	254.0
128.90	168.0
129.80	263.0
130.90	107.0
134.90	190.0
136.70	140.0
140.90	837.0
141.80	115.0
142.90	852.0
144.80	105.0
145.80	102.0
147.80	234.0
154.90	190.0
156.90	167.0
161.00	143.0
172.00	322.0
173.10	923.0
174.00	79568.0
175.00	6233.0
176.00	80032.0
177.00	5326.0
177.90	106.0
207.00	204.0
281.00	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	733.0
37.00	3980.0
38.00	3410.0
39.00	1307.0
40.00	292.0
41.00	169.0
42.90	116.0
44.00	953.0
45.00	756.0
47.00	930.0
48.00	522.0
49.00	3455.0
50.00	16015.0
51.00	5097.0
51.90	228.0
55.00	361.0
56.10	1210.0
57.00	2302.0
60.00	740.0
61.00	4677.0
62.00	3619.0
63.00	3008.0
64.00	254.0
65.00	161.0
66.90	206.0
68.00	8997.0
69.00	9694.0
70.00	630.0
72.00	415.0
73.10	4141.0
74.00	14943.0
75.00	45688.0
76.00	3757.0
77.00	635.0
78.00	354.0
78.90	2882.0
79.90	898.0
80.90	3093.0
81.90	617.0
83.00	144.0
85.90	209.0
87.00	3572.0
88.00	3453.0
90.90	353.0
92.00	2392.0
93.00	4274.0
94.00	10660.0
95.00	92224.0
96.10	6270.0
97.00	230.0
103.80	386.0
105.00	156.0
105.90	293.0
106.80	114.0
110.90	168.0
114.80	136.0
116.00	370.0
116.90	557.0
117.90	350.0
118.90	381.0
127.90	289.0
128.80	144.0
129.80	297.0
130.90	157.0
134.90	204.0
136.80	183.0
140.90	928.0
141.80	119.0
142.90	992.0
147.90	248.0
154.90	194.0
156.90	167.0
159.00	104.0
161.00	137.0
172.00	388.0
173.00	1043.0
174.00	86592.0
175.00	6554.0
176.00	86632.0
177.00	5365.0
177.80	154.0
207.00	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	643.0
37.00	3748.0
38.00	3296.0
39.00	1282.0
40.00	221.0
41.00	181.0
42.90	125.0
44.00	957.0
45.00	700.0
47.00	915.0
48.00	432.0
49.00	3077.0
50.00	14882.0
51.00	4883.0
51.90	220.0
55.00	320.0
56.10	1157.0
57.00	2133.0
60.00	826.0
61.00	4378.0
62.00	3587.0
63.00	2952.0
64.00	283.0
65.00	184.0
67.00	203.0
68.00	8765.0
69.00	8869.0
70.10	628.0
72.00	486.0
73.00	4311.0
74.00	13865.0
75.00	43160.0
76.00	3476.0
77.00	607.0
78.00	315.0
78.90	2667.0
79.90	911.0
80.90	2886.0
82.00	552.0
83.00	128.0
85.90	198.0
86.90	3415.0
88.00	3246.0
90.90	360.0
92.00	2445.0
93.00	4077.0
94.00	10274.0
95.00	88496.0
96.10	5895.0
97.00	214.0
103.80	349.0
104.80	138.0
105.90	308.0
110.80	161.0
114.80	123.0
116.00	284.0
117.00	583.0
117.80	335.0
118.90	314.0
127.90	320.0
128.90	125.0
129.90	281.0
130.90	164.0
134.90	205.0
136.90	202.0
139.90	103.0
140.90	921.0
141.80	108.0
142.90	1018.0
147.90	227.0
154.90	230.0
157.00	136.0
172.00	394.0
173.10	971.0
174.00	86160.0
175.00	6562.0
176.00	84256.0
177.00	5063.0
177.80	151.0
207.00	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44