


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU021820\
 Data File : VU036825.D
 Acq On : 18 Feb 2020 09:56
 Operator : JC/MD
 Sample : BFB09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB09

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR021220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Feb 19 04:53:41 2020

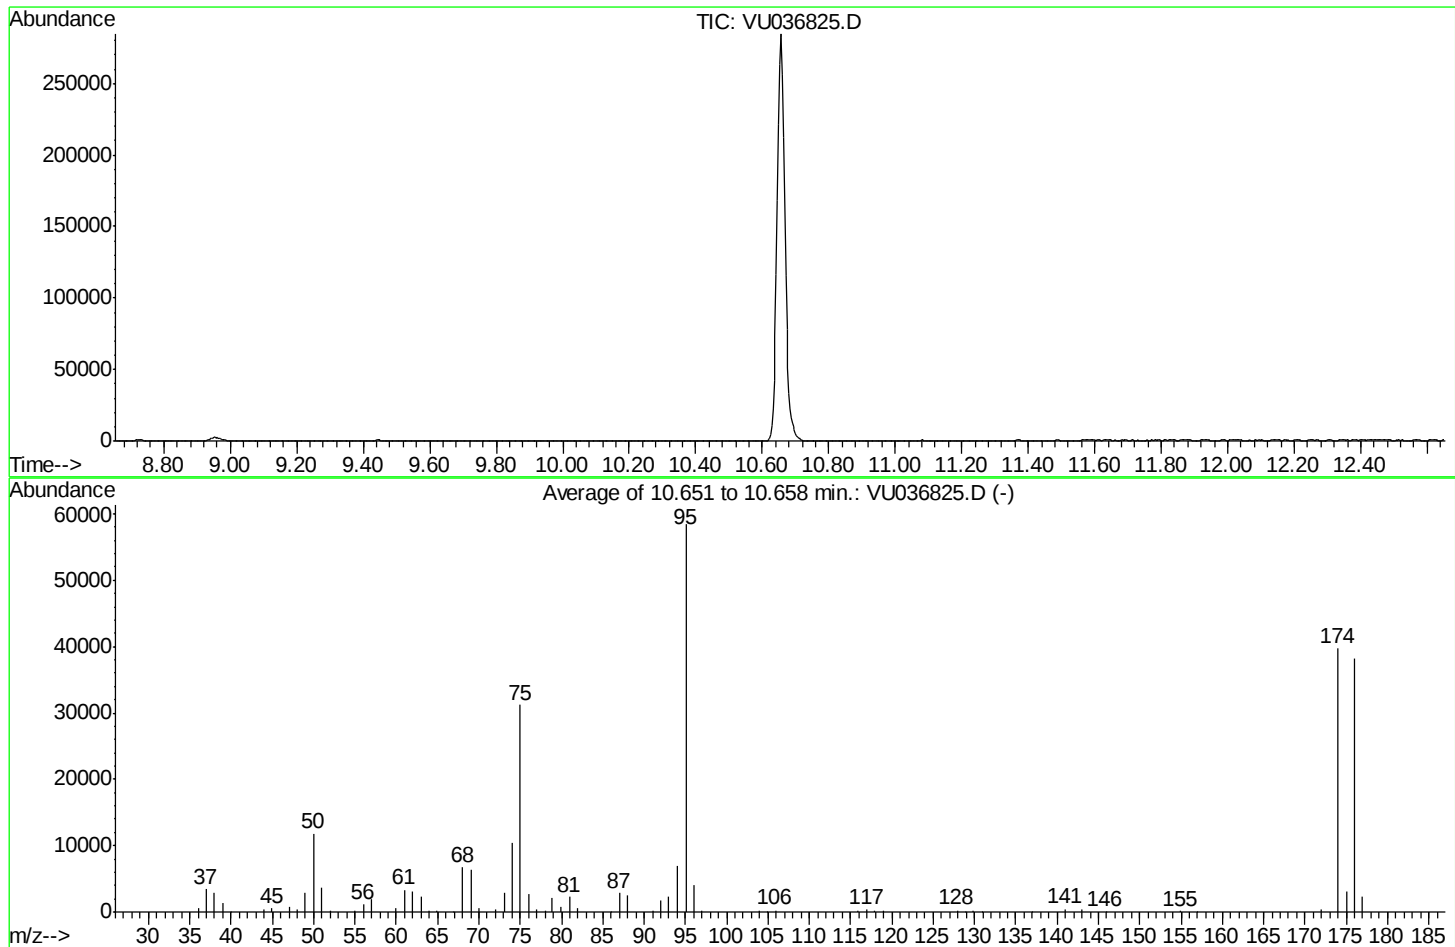

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	11811	PASS
75	95	30	80	53.4	31181	PASS
95	95	100	100	100.0	58421	PASS
96	95	5	9	6.8	3986	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.9	39696	PASS
175	174	5	9	7.9	3143	PASS
176	174	95	101	96.2	38176	PASS
177	176	5	9	6.1	2321	PASS

m/z	Abundance
36.00	729.0
37.00	3402.0
38.00	2872.0
39.00	1252.0
39.90	102.0
44.00	650.0
44.90	522.0
47.00	781.0
48.00	410.0
49.00	2761.0
50.00	11236.0
51.00	3319.0
52.00	169.0
54.90	202.0
56.00	1012.0
57.00	1786.0
60.00	624.0
61.00	3060.0
62.00	3041.0
63.10	2250.0
64.00	293.0
64.90	269.0
68.00	6462.0
69.00	6101.0
70.00	532.0
72.00	430.0
73.10	2731.0
74.00	10261.0
75.00	29576.0
76.00	2735.0
77.00	393.0
78.10	280.0
78.90	1985.0
79.90	729.0
80.90	2065.0
81.90	569.0
87.00	2811.0
88.00	2386.0
91.00	164.0
92.00	1595.0
93.00	2203.0
94.00	6859.0
95.00	56232.0
96.00	3840.0
97.00	148.0
103.90	249.0
104.90	106.0
105.90	265.0
115.90	206.0
117.00	375.0
117.90	251.0
118.90	262.0
127.90	186.0
129.80	138.0
141.00	432.0
143.00	395.0
155.00	115.0
157.00	105.0
172.00	287.0
174.00	37272.0
175.00	3053.0
176.00	35432.0
177.00	2130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	676.0
37.00	3562.0
38.00	3034.0
39.00	1326.0
43.90	695.0
44.90	597.0
47.00	742.0
48.00	431.0
49.00	3008.0
50.00	12053.0
51.00	3712.0
52.00	160.0
54.90	232.0
56.00	1113.0
57.00	2001.0
60.00	682.0
61.00	3446.0
62.00	3279.0
63.10	2512.0
64.00	288.0
64.90	262.0
66.90	147.0
68.00	6875.0
69.00	6428.0
70.00	531.0
72.00	441.0
73.00	2998.0
74.00	10793.0
75.00	32048.0
76.00	2792.0
77.00	430.0
78.10	267.0
78.90	2124.0
79.90	710.0
81.00	2318.0
81.90	568.0
87.00	2973.0
88.00	2631.0
91.00	200.0
92.00	1771.0
93.00	2437.0
94.10	7163.0
95.00	60200.0
96.00	4119.0
97.00	147.0
103.90	272.0
104.90	113.0
105.90	305.0
115.90	210.0
117.00	365.0
117.90	272.0
118.90	264.0
127.90	218.0
128.90	133.0
129.80	173.0
130.90	106.0
141.00	445.0
143.00	412.0
154.90	126.0
157.00	107.0
172.00	363.0
174.00	40960.0
175.00	3212.0
176.00	39296.0
177.00	2376.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	618.0
37.00	3296.0
38.00	2837.0
39.00	1370.0
44.00	702.0
45.00	579.0
47.10	643.0
48.00	430.0
49.00	2951.0
50.00	12145.0
51.00	3843.0
52.00	138.0
54.90	226.0
56.00	1125.0
57.00	2048.0
60.00	695.0
61.00	3388.0
62.00	3246.0
63.10	2475.0
64.00	285.0
65.00	242.0
66.90	151.0
68.00	6653.0
69.00	6335.0
70.00	496.0
72.00	456.0
73.00	2965.0
74.00	10465.0
75.00	31920.0
76.00	2639.0
76.90	420.0
78.00	254.0
78.90	2155.0
80.00	655.0
81.00	2452.0
81.90	530.0
85.90	104.0
87.00	2700.0
88.00	2662.0
91.00	208.0
92.00	1666.0
93.00	2515.0
94.10	7020.0
95.10	58832.0
96.00	3999.0
97.00	134.0
103.90	266.0
105.90	314.0
115.90	192.0
117.00	376.0
117.90	253.0
118.90	263.0
127.90	212.0
128.90	139.0
129.80	166.0
137.00	108.0
141.00	443.0
143.00	422.0
145.90	107.0
155.00	100.0
171.90	399.0
174.00	40856.0
175.00	3165.0
176.00	39800.0
177.00	2459.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
43.90	355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09