

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021821\
 Data File : VU042341.D
 Acq On : 18 Feb 2021 10:54
 Operator : SY/MD
 Sample : VU0218WBL05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0218WBL05

Quant Time: Feb 19 03:07:38 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 19 02:55:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.382	168	147501	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	217586	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.427	117	194174	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	92752	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.713	65	103625	46.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.66%	
35) Dibromofluoromethane	5.301	113	73590	47.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.84%	
50) Toluene-d8	7.906	98	266306	48.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.84%	
62) 4-Bromofluorobenzene	10.639	95	96032	44.30	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.60%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021821\
Data File : VU042341.D
Acq On : 18 Feb 2021 10:54
Operator : SY/MD
Sample : VU0218WBL05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0218WBL05

Quant Time: Feb 19 03:07:38 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 19 02:55:52 2021
Response via : Initial Calibration




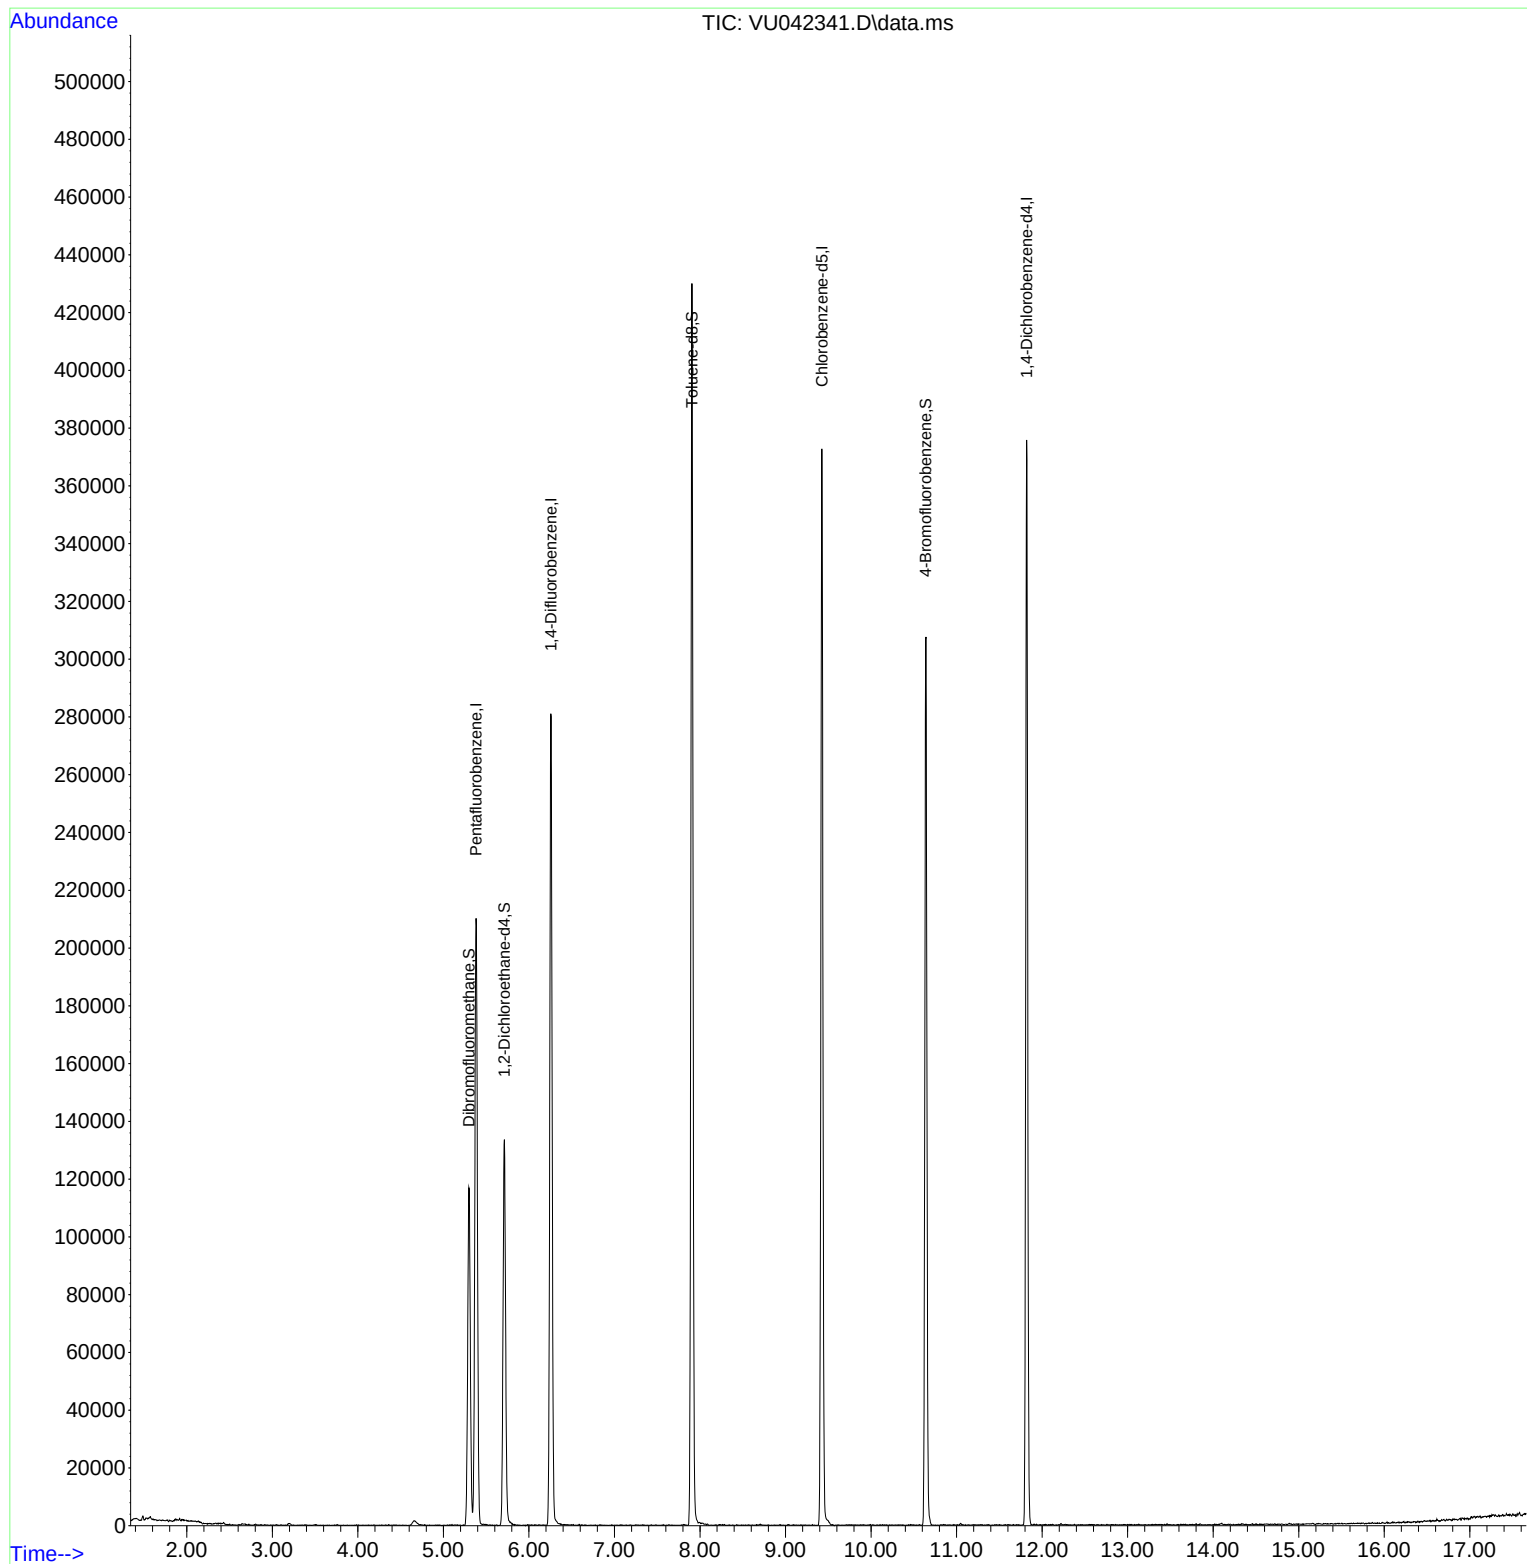


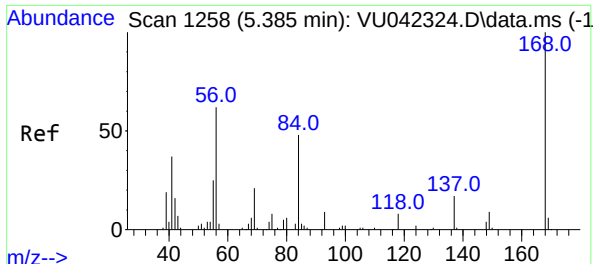

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.003 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54




Instrument :
MSVOA_U
ClientSampleId :
VU0218WBL05


Tgt Ion:168 Resp: 147501
Ion Ratio Lower Upper
168 100
99 57.7 45.0 67.4

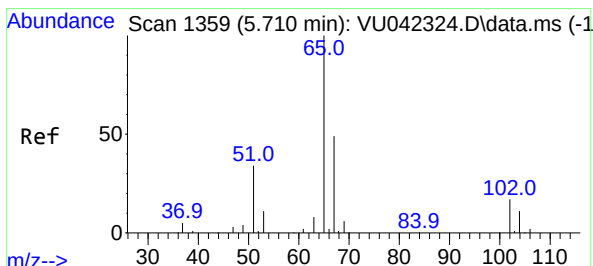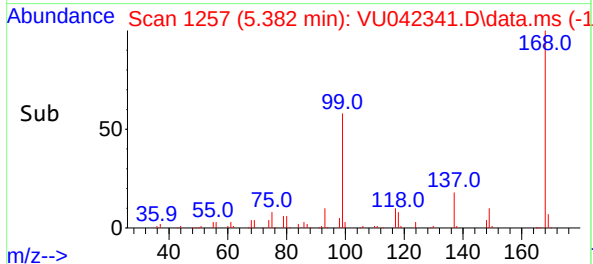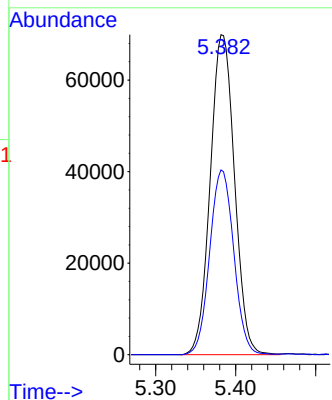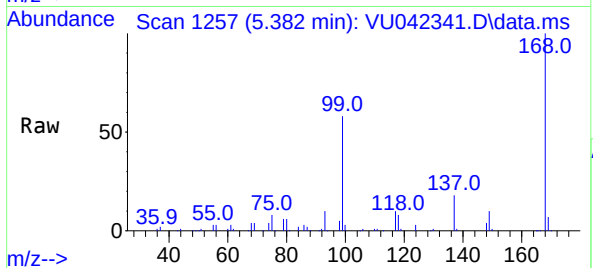

#33
1,2-Dichloroethane-d4
Concen: 46.33 ug/l
RT: 5.713 min Scan# 1360
Delta R.T. 0.003 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54

Tgt Ion: 65 Resp: 103625
Ion Ratio Lower Upper
65 100
67 51.3 0.0 99.8


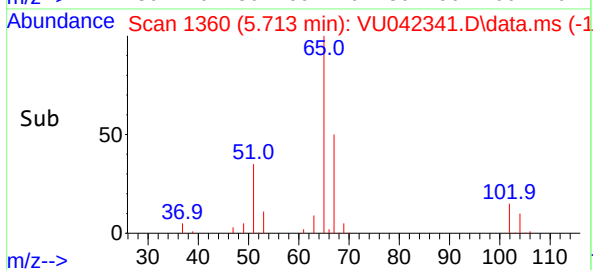
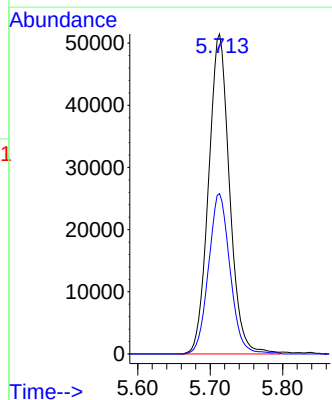
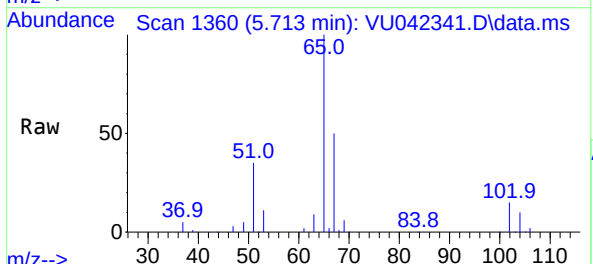


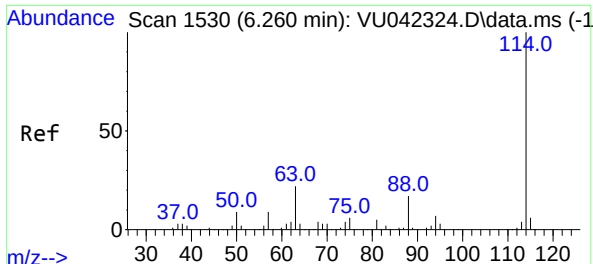

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. -0.003 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54




Instrument :
MSVOA_U
ClientSampleId :
VU0218WBL05


Tgt Ion:114 Resp: 217586
Ion Ratio Lower Upper
114 100
63 22.7 0.0 44.2
88 15.9 0.0 33.4

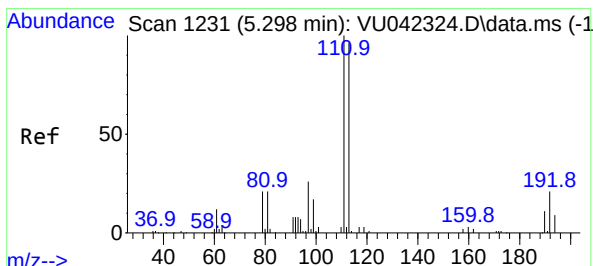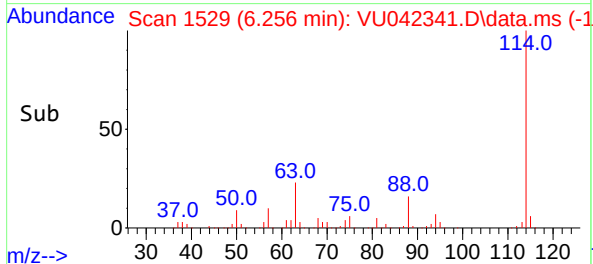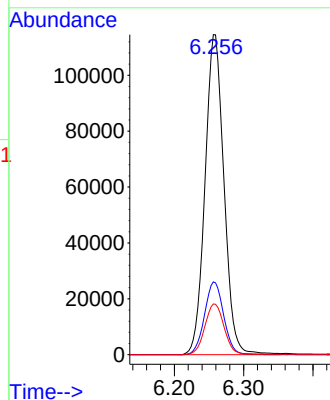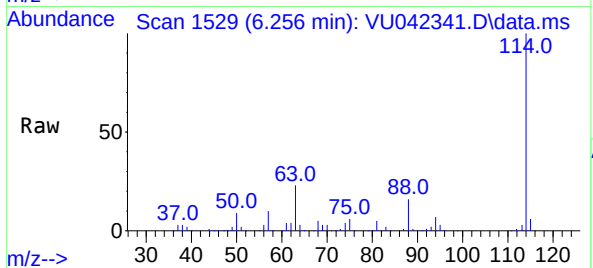

#35
Dibromofluoromethane
Concen: 47.92 ug/l
RT: 5.301 min Scan# 1232
Delta R.T. 0.003 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54

Tgt Ion:113 Resp: 73590
Ion Ratio Lower Upper
113 100
111 102.2 81.8 122.8
192 21.7 17.2 25.8


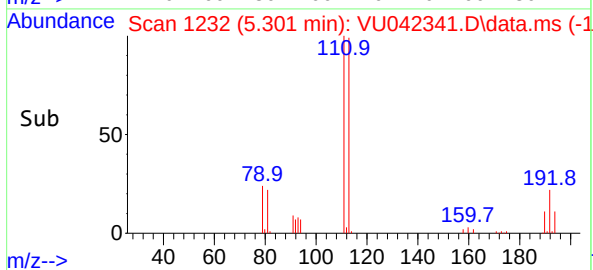
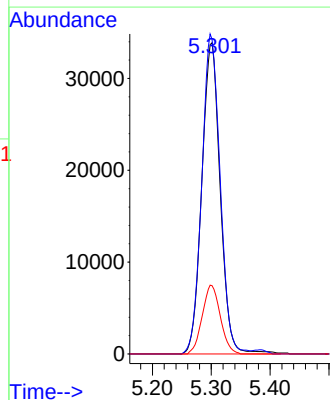
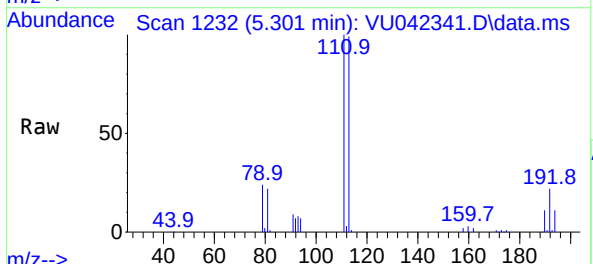


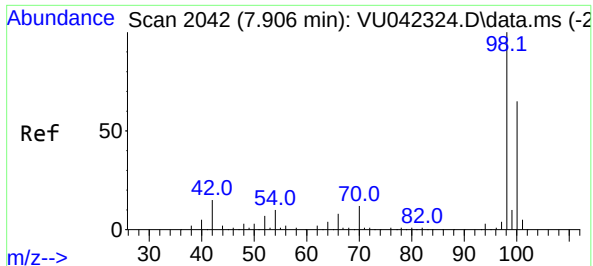

#50
Toluene-d8
Concen: 48.42 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54




Instrument :
MSVOA_U
ClientSampleId :
VU0218WBL05


Tgt Ion: 98 Resp: 266306
Ion Ratio Lower Upper
98 100
100 63.4 50.2 75.2

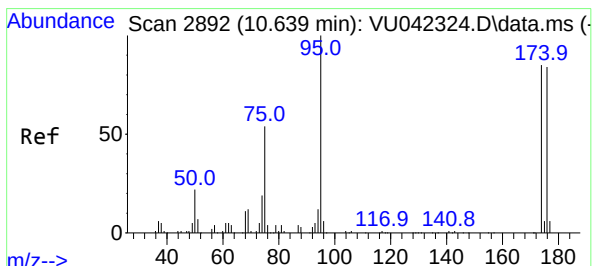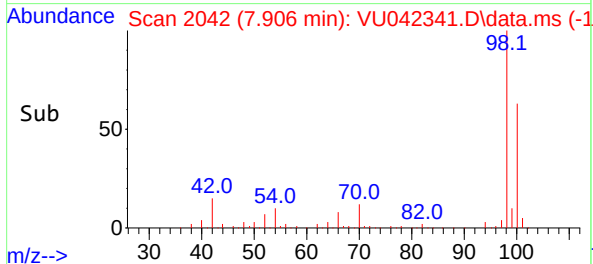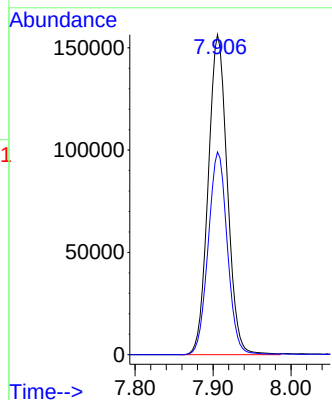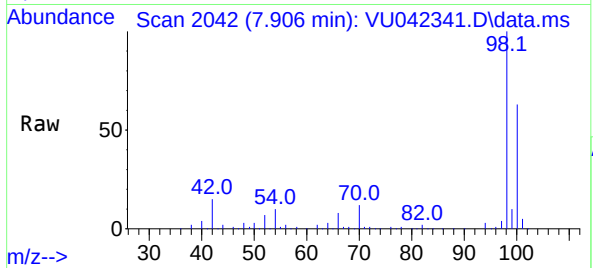

#62
4-Bromofluorobenzene
Concen: 44.30 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54

Tgt Ion: 95 Resp: 96032
Ion Ratio Lower Upper
95 100
174 87.2 0.0 172.2
176 83.8 0.0 168.8


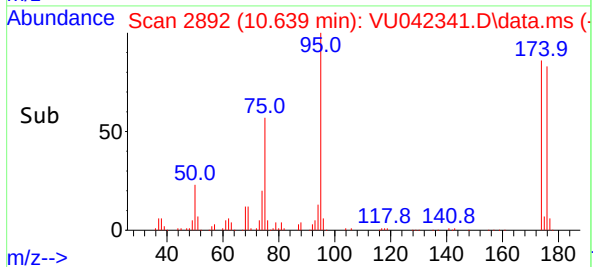
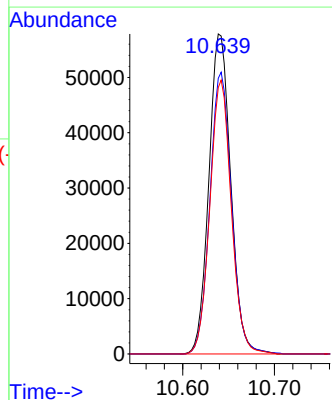
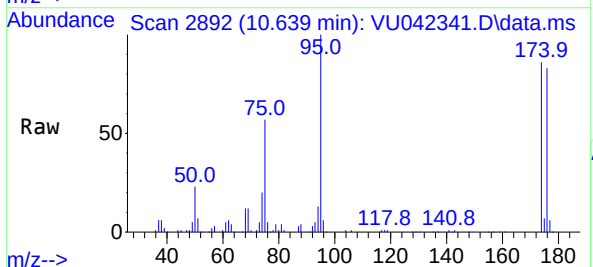


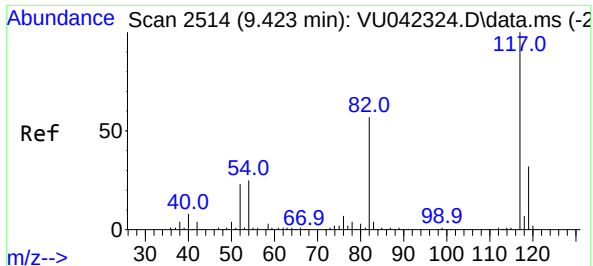

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.427 min Scan# 2515
Delta R.T. 0.003 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54

Instrument :
MSVOA_U
ClientSampleId :
VU0218WBL05

Tgt Ion:117 Resp: 194174
Ion Ratio Lower Upper
117 100
82 56.8 45.8 68.6
119 32.2 25.8 38.8

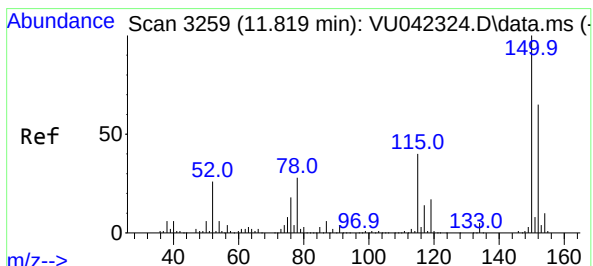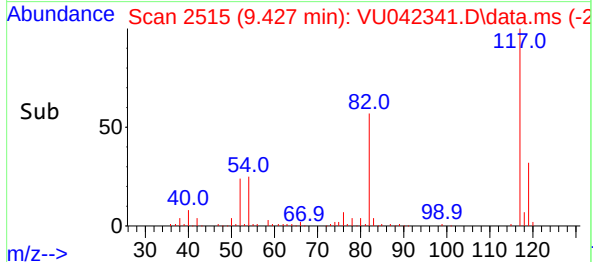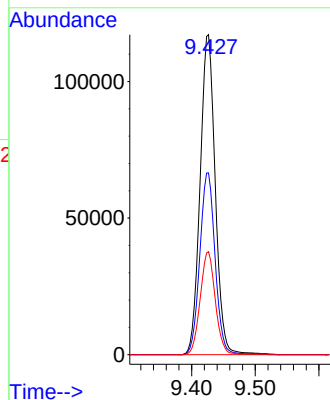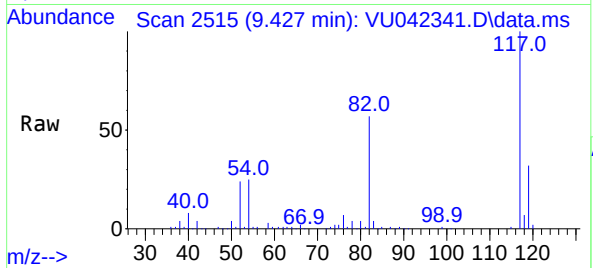

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU042341.D
Acq: 18 Feb 2021 10:54

Tgt Ion:152 Resp: 92752
Ion Ratio Lower Upper
152 100
115 59.0 41.5 124.6
150 160.9 0.0 342.4

