


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021821\
 Data File : VU042337.D
 Acq On : 18 Feb 2021 08:56
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U021721W.M
 Title : SW846 8260
 Last Update : Fri Feb 19 02:55:52 2021

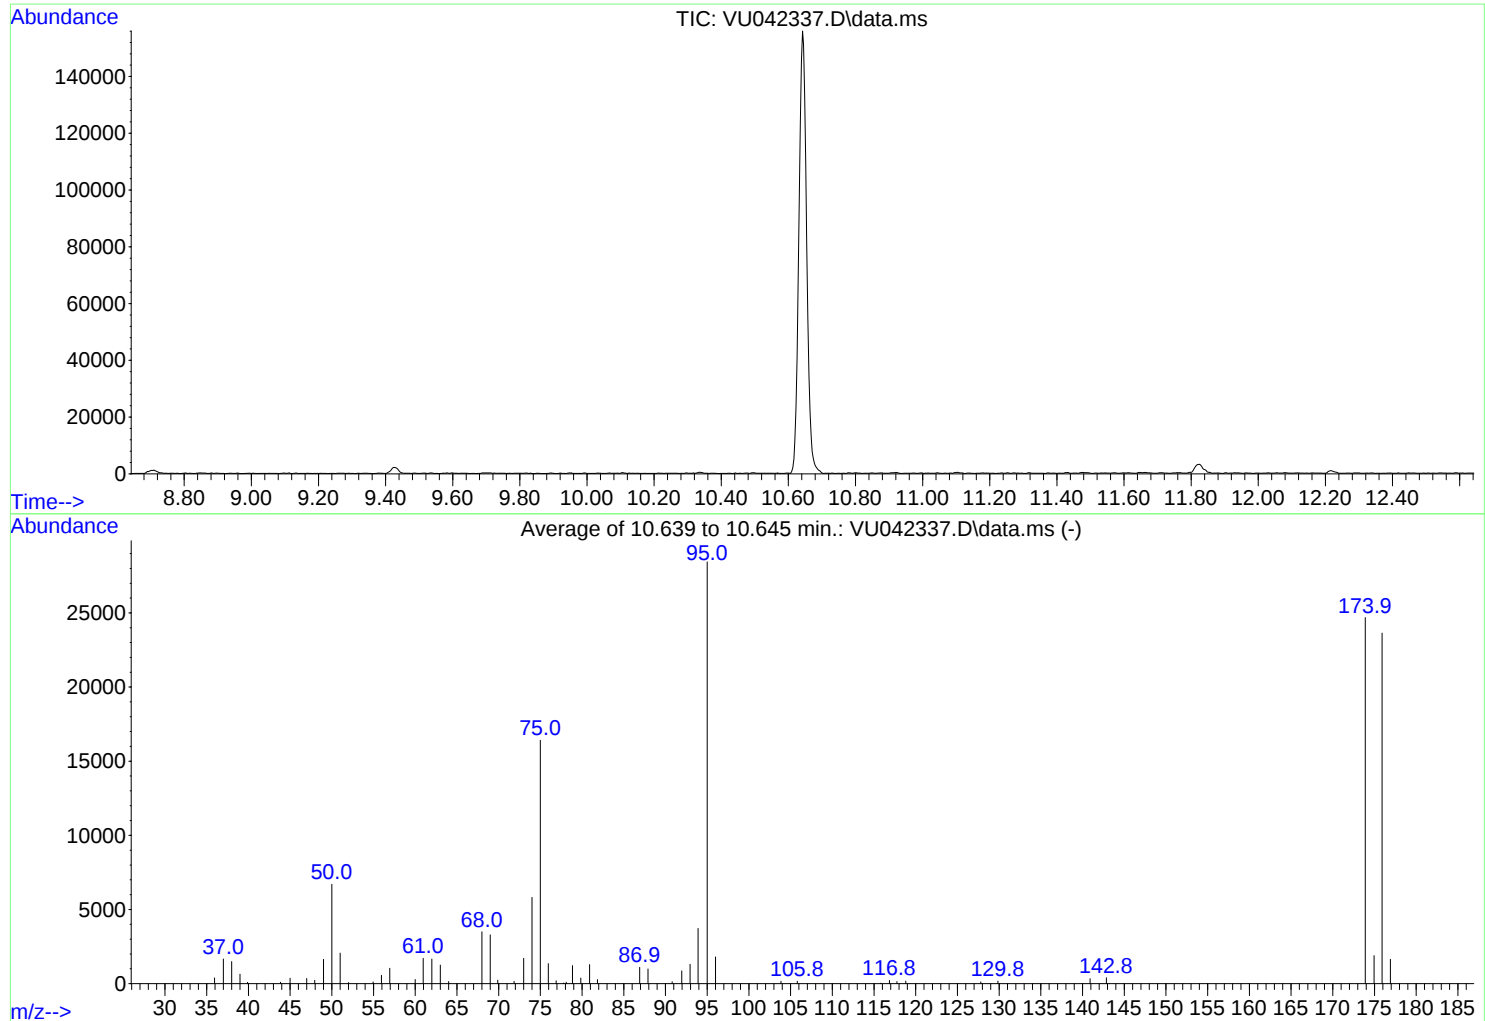

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	6698	PASS
75	95	30	60	57.7	16410	PASS
95	95	100	100	100.0	28443	PASS
96	95	5	9	6.3	1806	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.8	24691	PASS
175	174	5	9	7.6	1884	PASS
176	174	95	101	95.7	23635	PASS
177	176	5	9	7.0	1643	PASS