

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021822\
 Data File : VU047209.D
 Acq On : 17 Feb 2022 17:08
 Operator : SY/MD
 Sample : N1558-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M84

Quant Time: Feb 18 03:34:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 18 03:32:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	169844	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	175187	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	98286	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	58374	4.069	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.400%
7) Chloroethane-d5	1.919	69	50284	4.423	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.400%
11) 1,1-Dichloroethene-d2	2.572	65	23614	3.980	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.600%
20) 2-Butanone-d5	4.636	46	166305	48.505	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.020%
24) Chloroform-d	5.067	84	106433	4.467	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
26) 1,2-Dichloroethane-d4	5.707	65	57080	4.308	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.200%
32) Benzene-d6	5.732	84	218700	4.468	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
36) 1,2-Dichloropropane-d6	6.694	67	69931	4.490	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.800%
41) Toluene-d8	7.903	98	208405	4.352	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.000%
43) trans-1,3-Dichloroprop...	8.182	79	28071	3.976	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.600%
46) 2-Hexanone-d5	8.636	63	140675	37.840	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.680%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	55695	3.934	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.600%
66) 1,2-Dichlorobenzene-d4	12.195	152	81572	4.626	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%
Target Compounds						
					Qvalue	
13) Acetone	2.655	43	40538	23.618	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021822\
Data File : VU047209.D
Acq On : 17 Feb 2022 17:08
Operator : SY/MD
Sample : N1558-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M84


Quant Time: Feb 18 03:34:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 18 03:32:37 2022
Response via : Initial Calibration

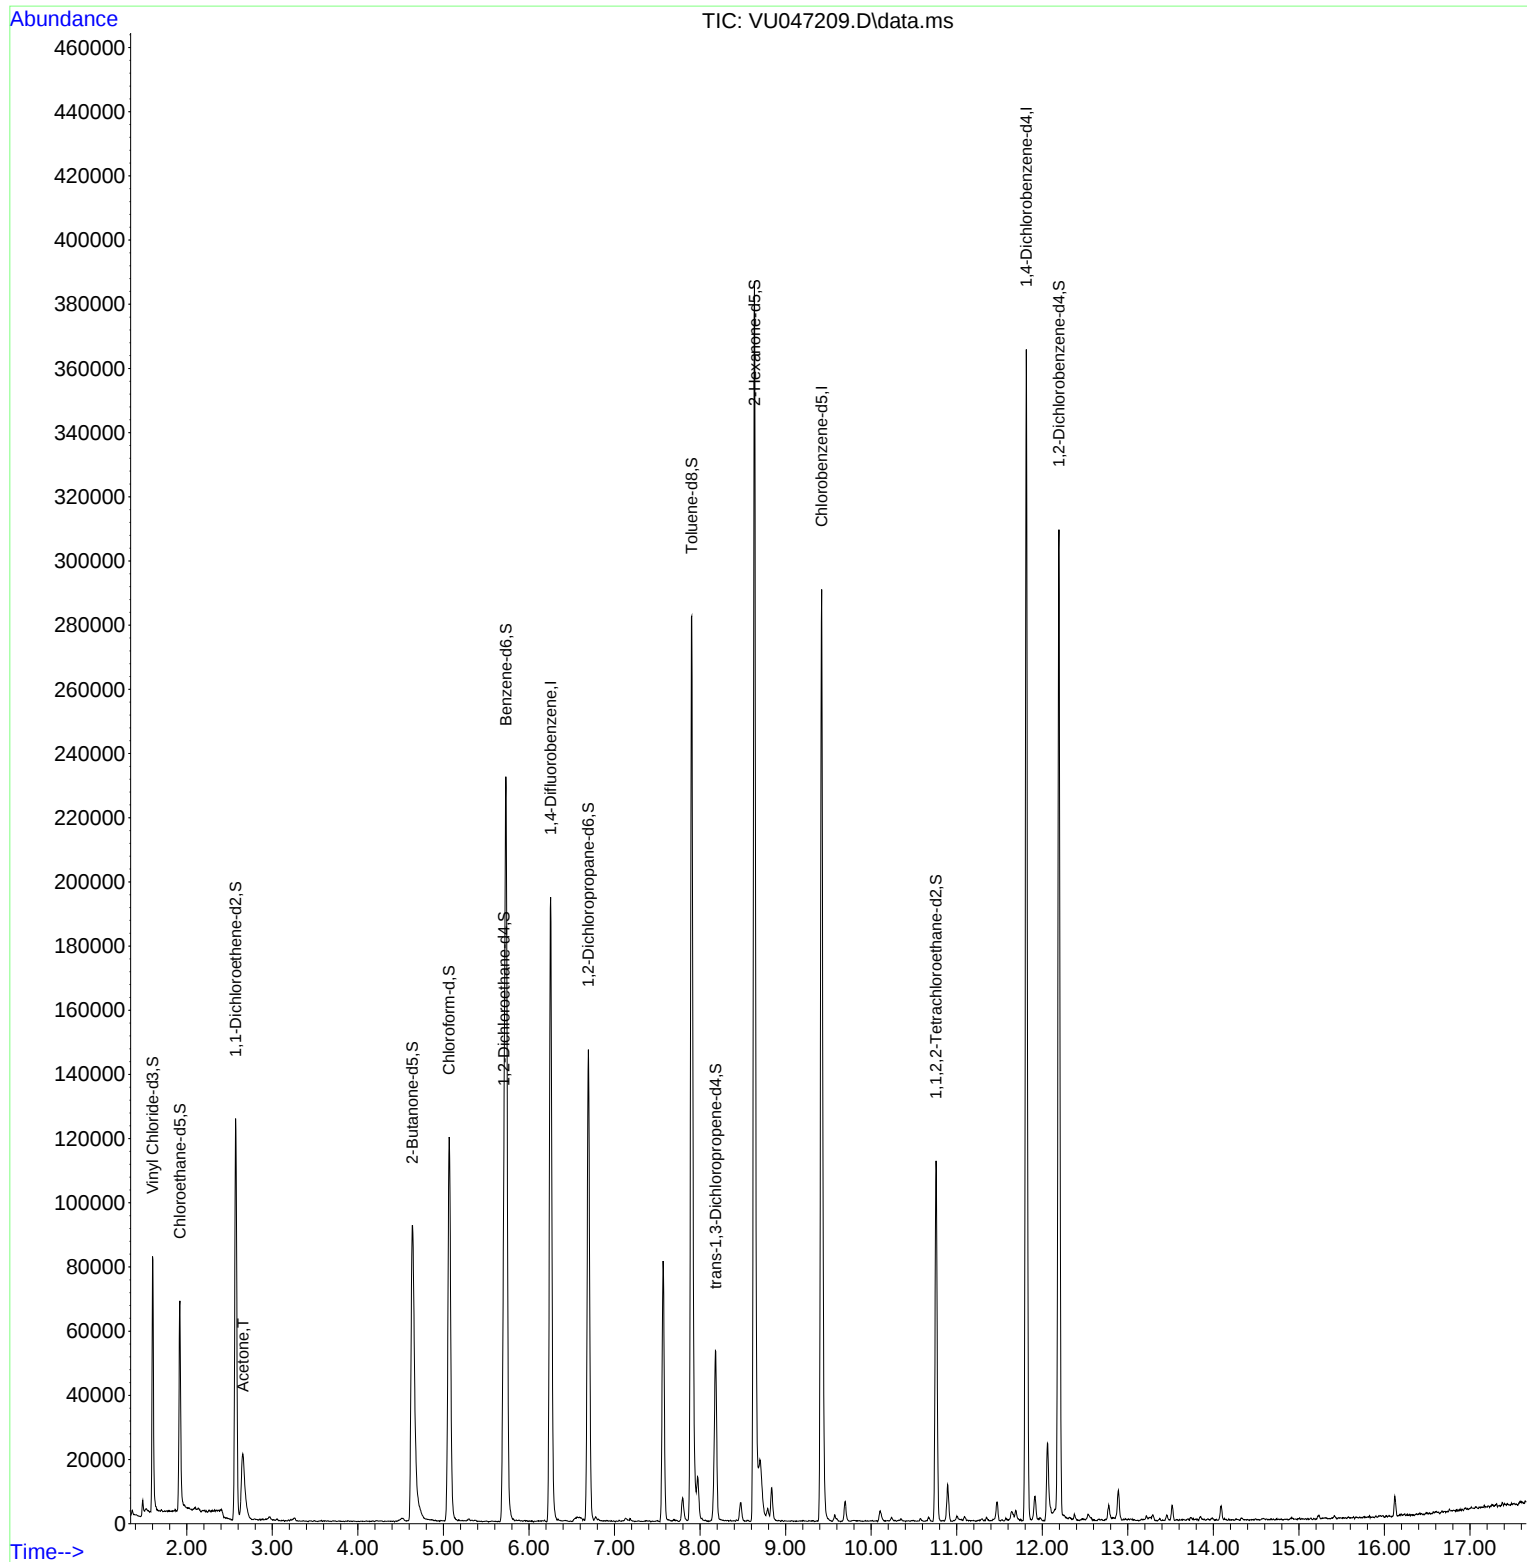

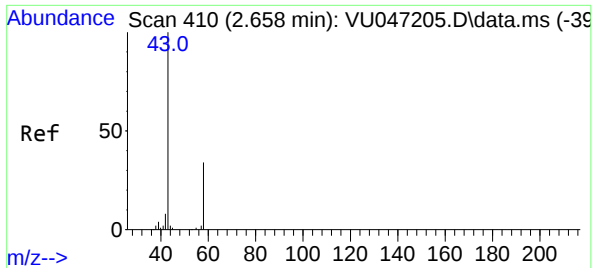

#13
Acetone
Concen: 23.618 ug/L
RT: 2.655 min Scan# 409
Delta R.T. -0.003 min
Lab File: VU047209.D
Acq: 17 Feb 2022 17:08

Instrument :
MSVOA_U
ClientSampleId :
F4M84

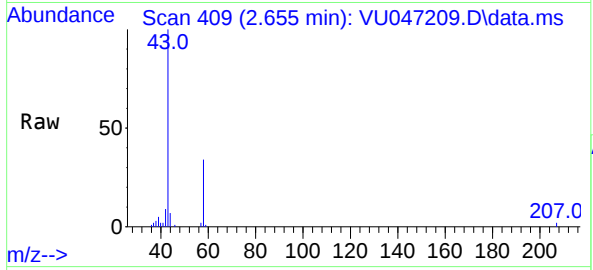

Tgt Ion: 43 Resp: 40538
Ion Ratio Lower Upper
43 100
58 33.2 0.0 71.6

